
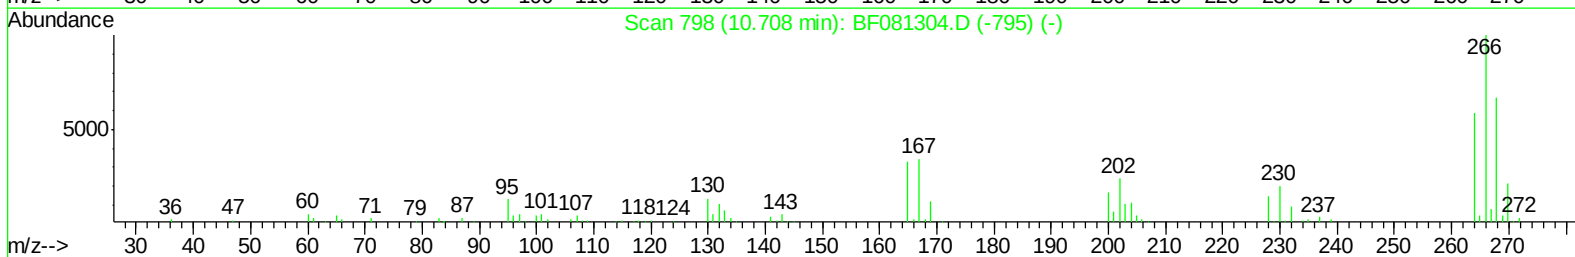
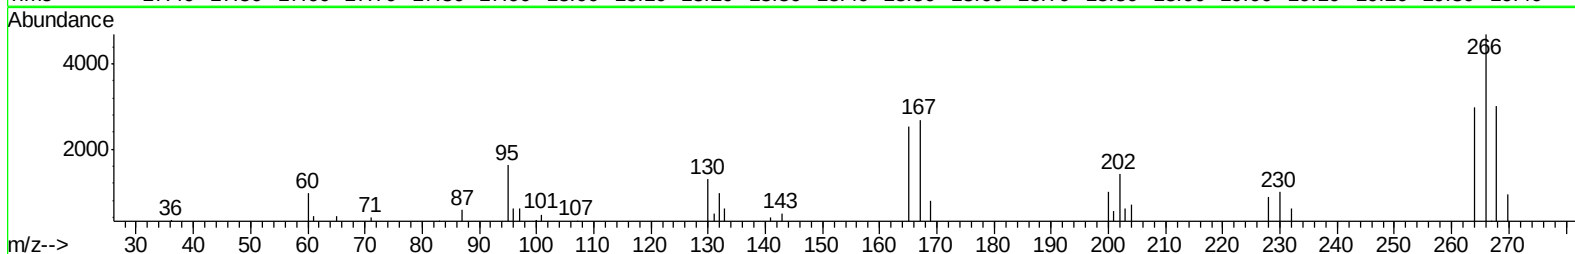


Data Path : Z:\HPCHEM1\BNA_F\Data\BF091715\
Data File : BF081674.D
Acq On : 17 Sep 2015 11:40
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 06:53:47 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 15 14:03:59 2015
Response via : Initial Calibration

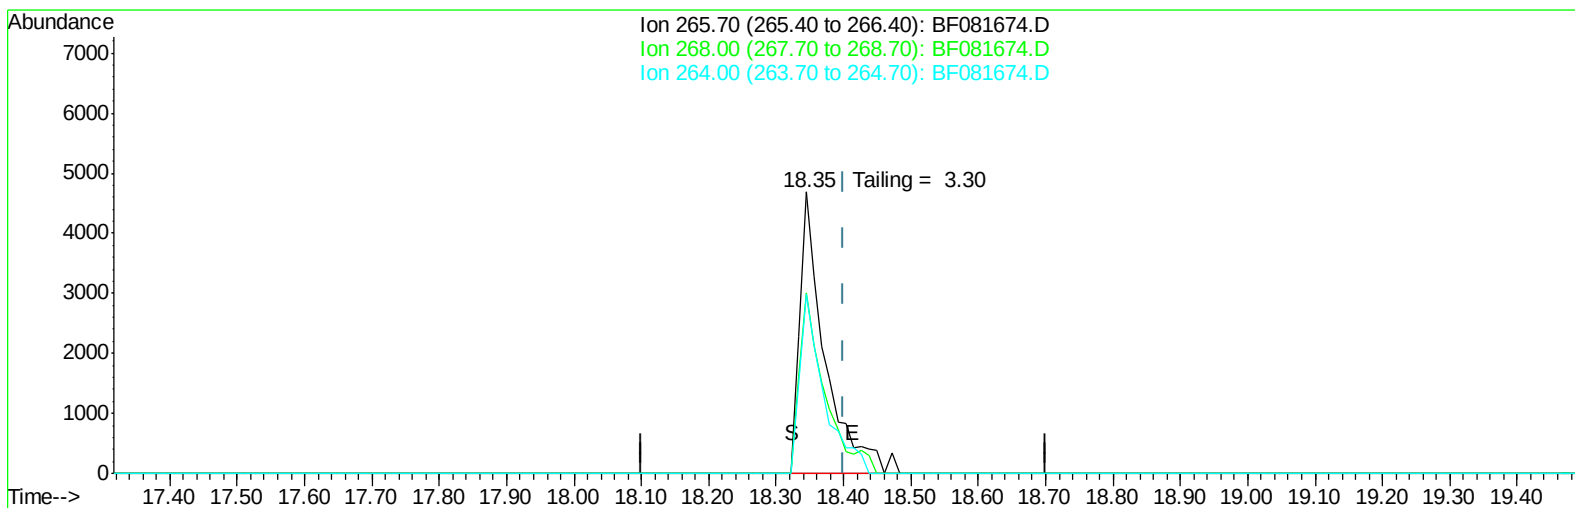

TIC: BF081674.D

(69) Pentachlorophenol (C)




18.346min (-0.056) 0.00ng

response 12107

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	64.29
264.00	62.70	63.84
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF091715\
Data File : BF081674.D
Acq On : 17 Sep 2015 11:40
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 06:53:47 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 15 14:03:59 2015
Response via : Initial Calibration

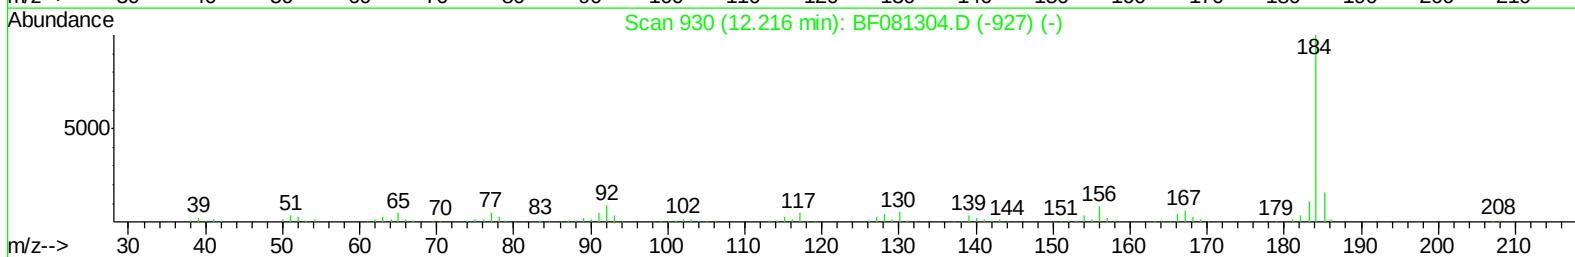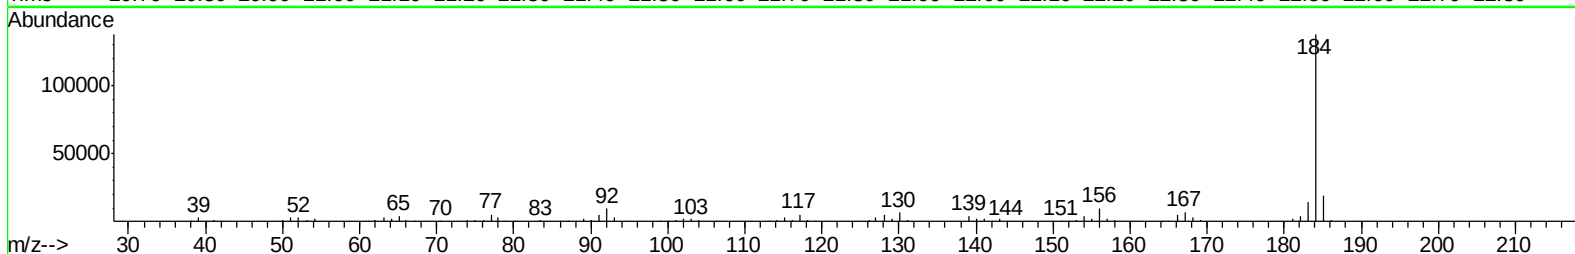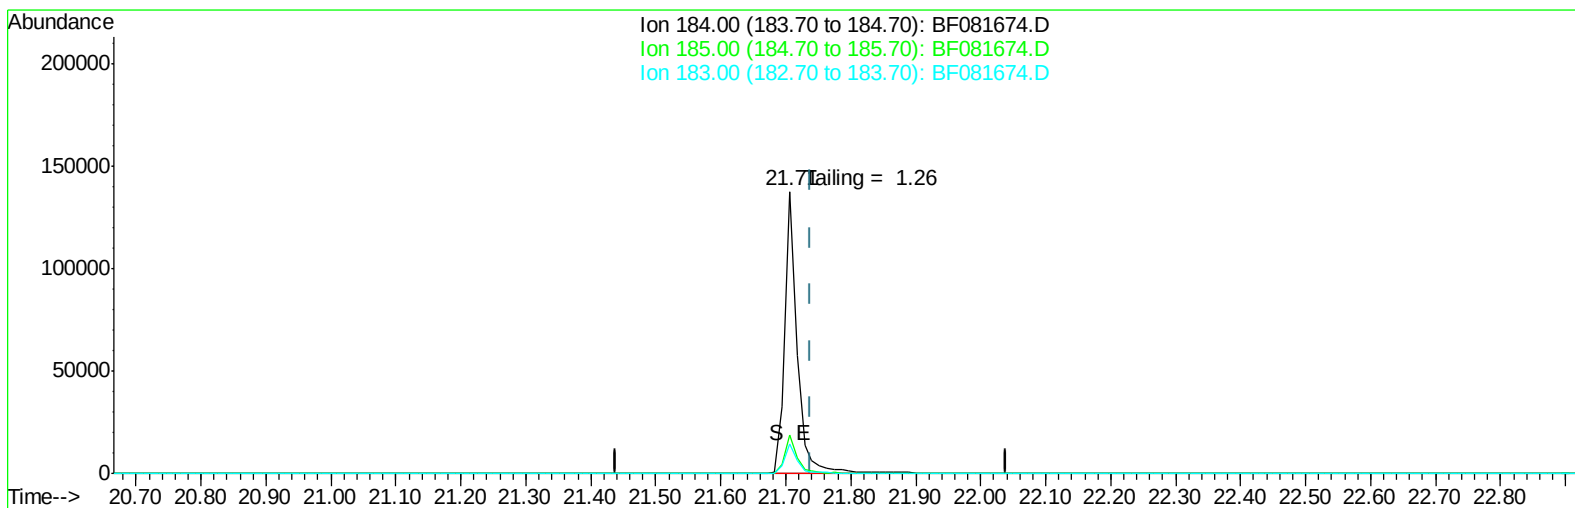

TIC: BF081674.D

(76) Benzidine

21.706min (-0.033) 0.00ng

response 181931

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.76
183.00	9.50	10.30
0.00	0.00	0.00