


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091715\
 Data File : BF081674.D
 Acq On : 17 Sep 2015 11:40
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 15 14:03:59 2015

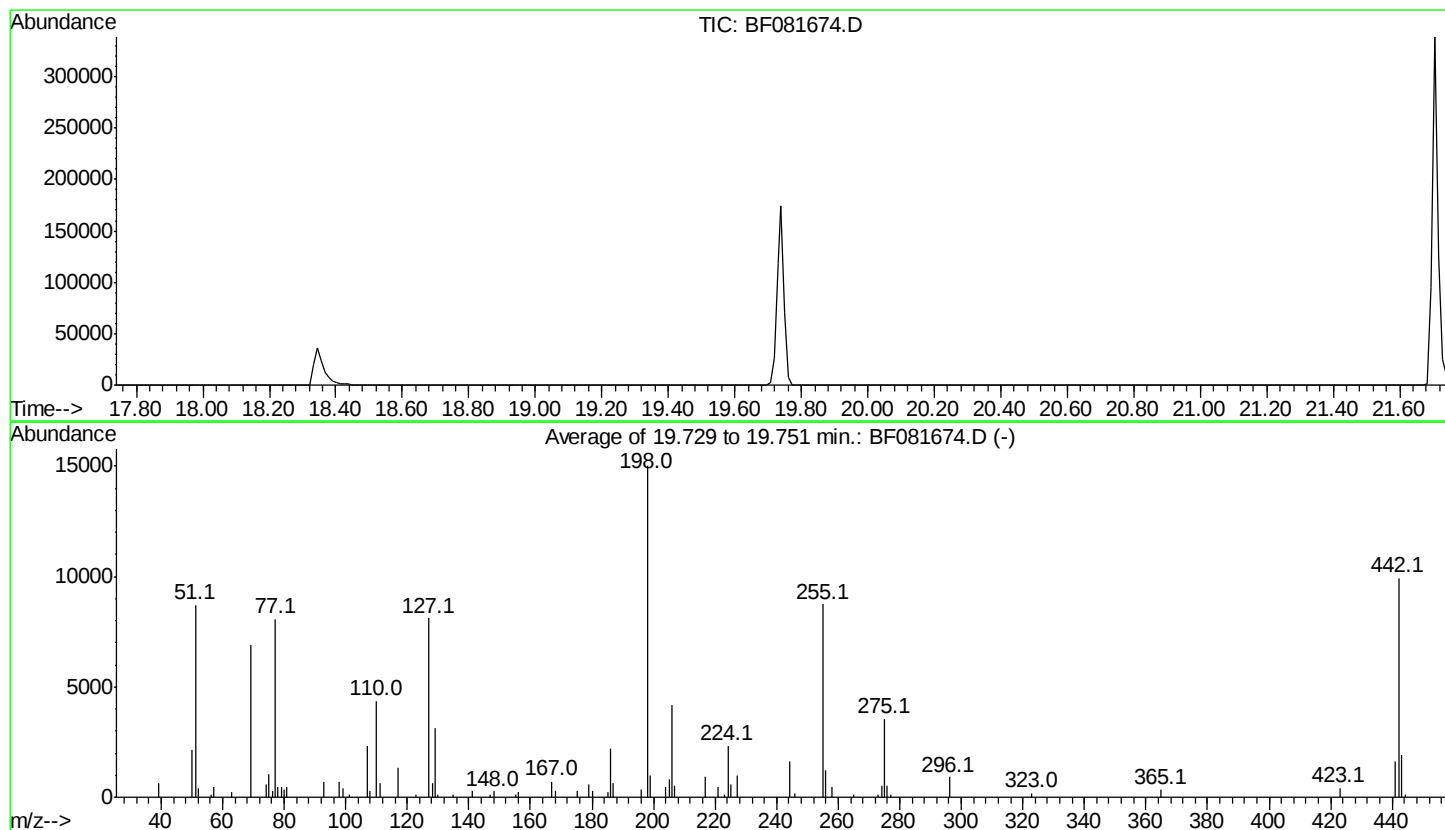

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.0	8712	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.1	6922	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.9	8104	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	15026	PASS
199	198	5	9	6.5	976	PASS
275	198	10	60	23.6	3552	PASS
365	198	1	100	2.2	338	PASS
441	442	0.01	24	16.5	1637	PASS
442	198	50	100	66.1	9930	PASS
443	442	15	24	19.3	1913	PASS