
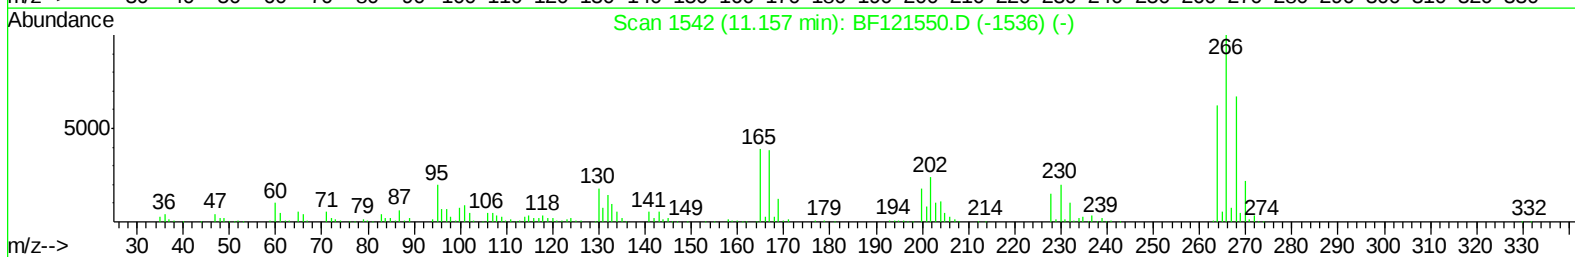
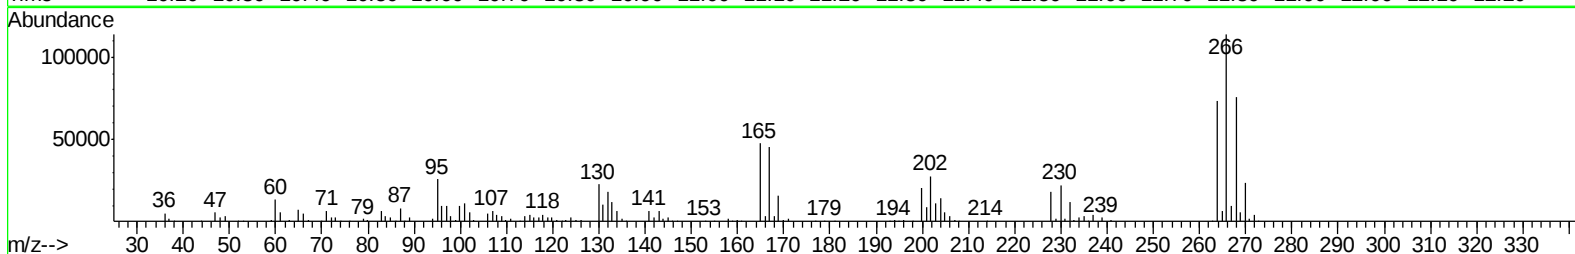


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091720\
Data File : BF121597.D
Acq On : 17 Sep 2020 14:28
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 02:51:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 10 16:47:54 2020
Response via : Initial Calibration

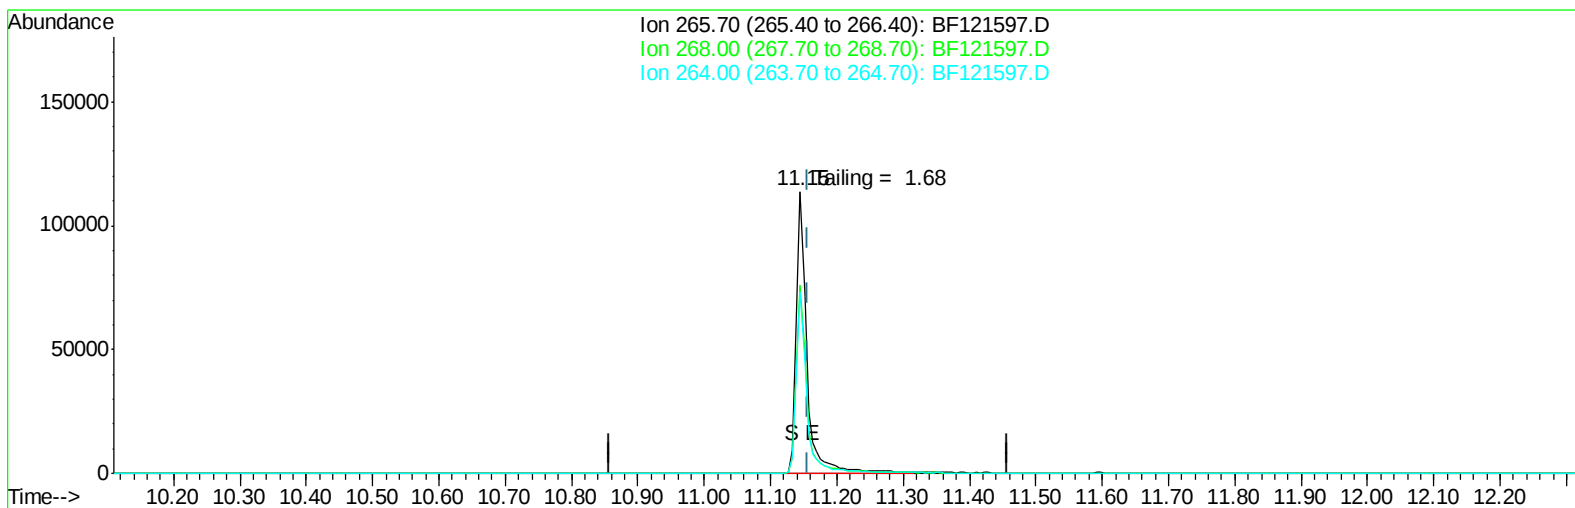

TIC: BF121597.D

(70) Pentachlorophenol (C)




11.145min (-0.012) 43428.95ng

response 121355

Ion	Exp%	Act%
265.70	100	100
268.00	66.90	66.75
264.00	62.30	64.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091720\
 Data File : BF121597.D
 Acq On : 17 Sep 2020 14:28
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 02:51:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 10 16:47:54 2020
 Response via : Initial Calibration

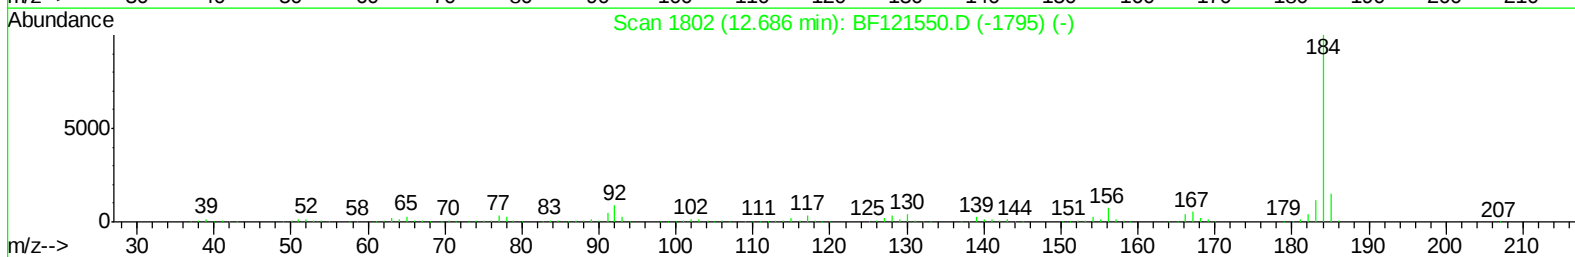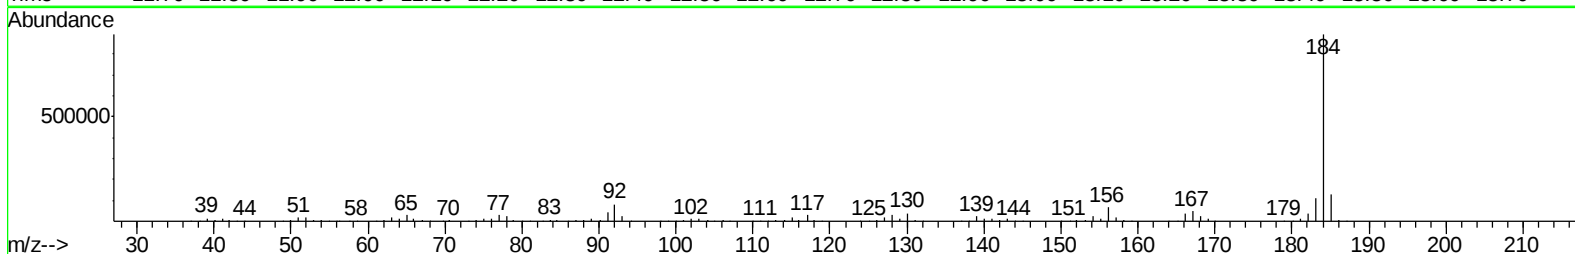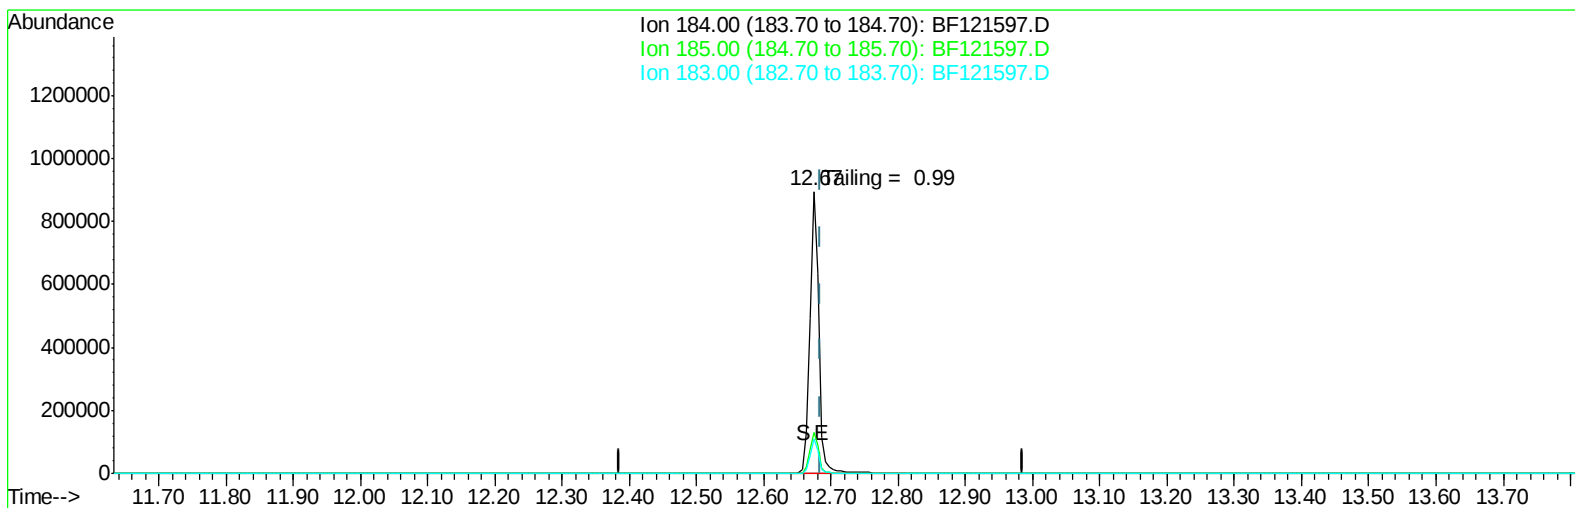

TIC: BF121597.D

(77) Benzidine

12.674min (-0.012) 0.00ng

response 848771

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.75
183.00	11.90	12.14
0.00	0.00	0.00