

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091815\
 Data File : BF081705.D
 Acq On : 18 Sep 2015 19:55
 Operator : UM/IZ
 Sample : G3704-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-11-9-15-15

Quant Time: Sep 18 23:02:07 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 15 14:03:59 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	44608	20.00	ng	-0.06
21) Naphthalene-d8	11.06	136	171702	20.00	ng	-0.06
38) Acenaphthene-d10	15.19	164	84133	20.00	ng	-0.07
63) Phenanthrene-d10	18.70	188	174670	20.00	ng	-0.06
75) Chrysene-d12	23.34	240	137655	20.00	ng	-0.04
86) Perylene-d12	24.78	264	96336	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	164924	57.36	ng	-0.03
7) Phenol-d6	7.58	99	134385	35.31	ng	-0.07
23) Nitrobenzene-d5	9.46	82	405043	113.81	ng	-0.07
41) 2,4,6-Tribromophenol	17.10	330	128118	171.02	ng	-0.07
44) 2-Fluorobiphenyl	13.72	172	714877	108.89	ng	-0.06
78) Terphenyl-d14	22.07	244	597960	101.12	ng	-0.04
Target Compounds						
2) 1,4-Dioxane	1.53	88	17909	13.87	ng	# 11
15) Benzyl Alcohol	8.49	79	6623	2.12	ng	# 27
19) n-Nitroso-di-n-propylamine	9.46	70	52519	20.28	ng	# 69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091815\
Data File : BF081705.D
Acq On : 18 Sep 2015 19:55
Operator : UM/IZ
Sample : G3704-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-11-9-15-15

Quant Time: Sep 18 23:02:07 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 15 14:03:59 2015
Response via : Initial Calibration

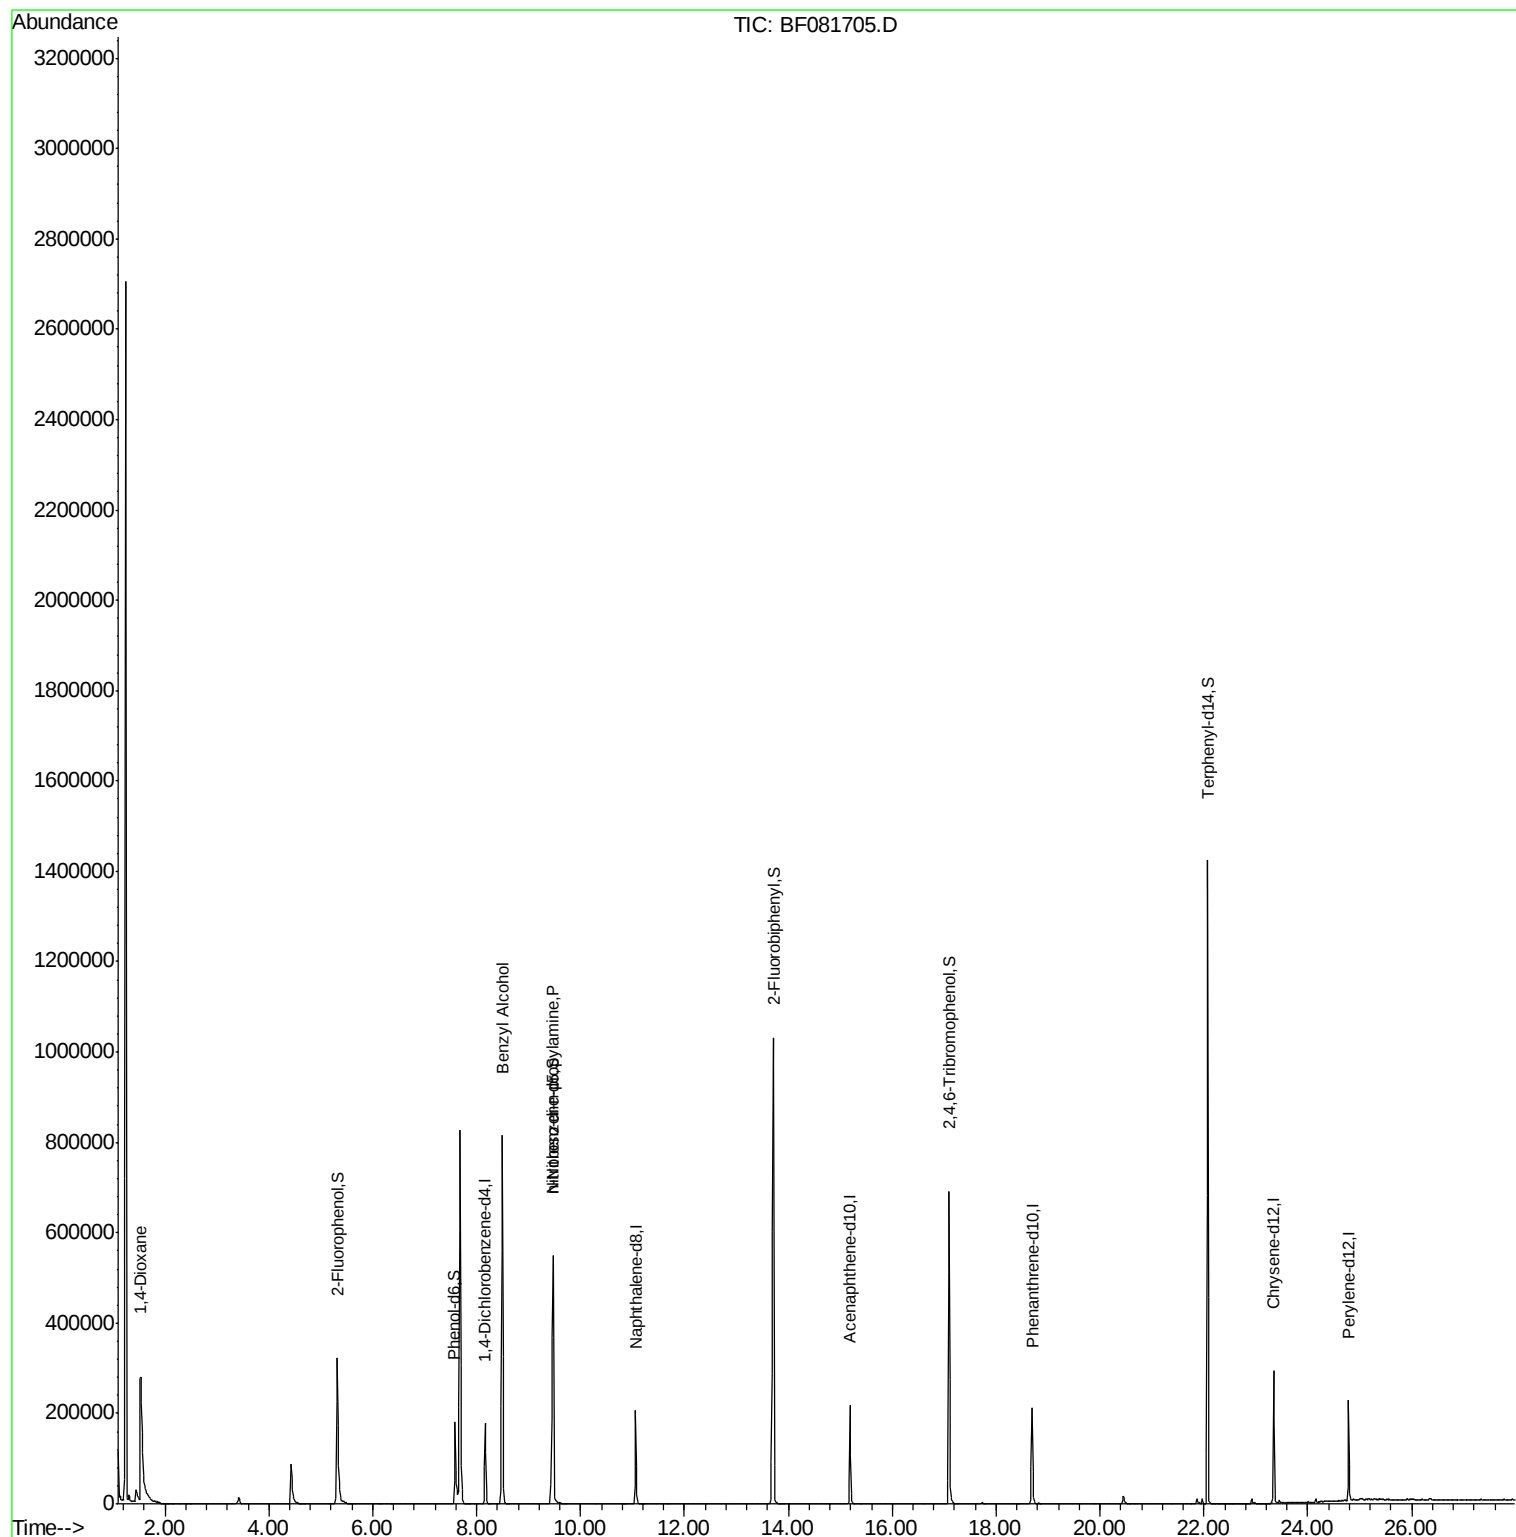



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.16 min Scan# 619

Delta R.T. -0.06 min

Lab File: BF081705.D

Acq: 18 Sep 2015 19:55

Instrument :

BNA_F

ClientSampleId :

MW-11-9-15-15


Tgt Ion:152 Resp: 44608

Ion Ratio Lower Upper

152 100

150 160.3 124.7 187.1




115 69.9 39.0 58.4#

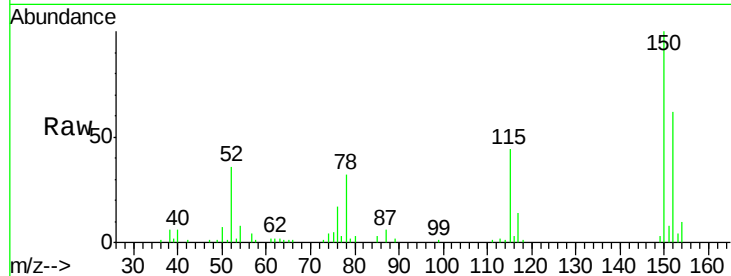

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

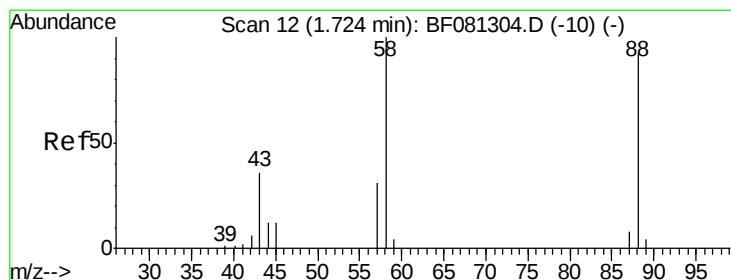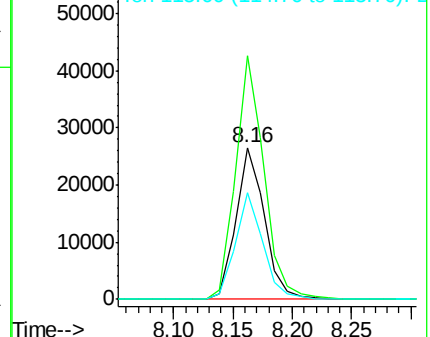

#2

1,4-Dioxane

Concen: 13.87 ng

RT: 1.53 min Scan# 39

Delta R.T. -0.03 min

Lab File: BF081705.D

Acq: 18 Sep 2015 19:55


Tgt Ion: 88 Resp: 17909

Ion Ratio Lower Upper

88 100

58 0.0 77.7 116.5#



43 0.0 26.6 40.0#

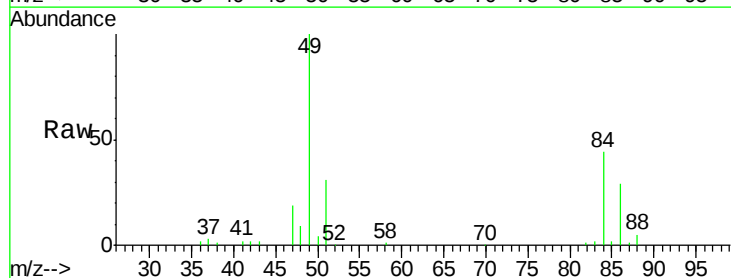


Abundance Ion 88.00 (87.70 to 88.70): BF0

Ion 58.00 (57.70 to 58.70): BF0

Ion 43.00 (42.70 to 43.70): BF0

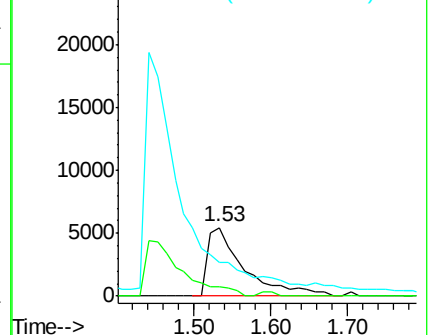







#5
 2-Fluorophenol
 Concen: 57.36 ng
 RT: 5.32 min Scan# 370
 Delta R.T. -0.03 min
 Lab File: BF081705.D
 Acq: 18 Sep 2015 19:55

Instrument :
 BNA_F
 ClientSampleId :
 MW-11-9-15-15

Tgt Ion: 112 Resp: 164924
 Ion Ratio Lower Upper
 112 100
 64 74.7 39.7 59.5#
 63 42.1 17.4 26.0#

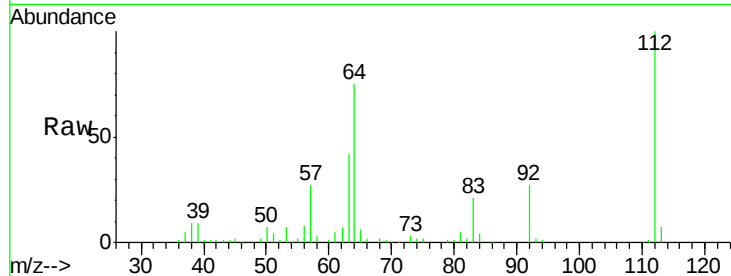


Abundance Ion 112.00 (111.70 to 112.70): B
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

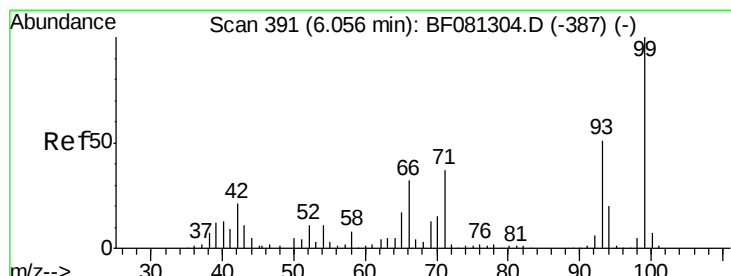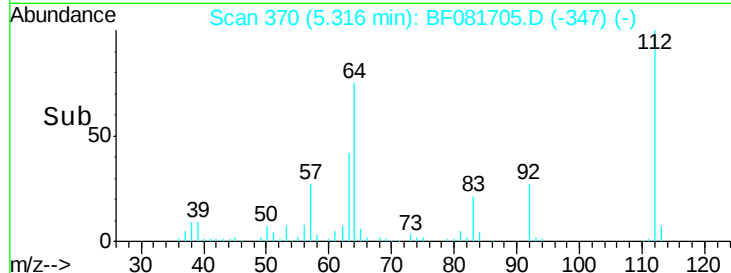
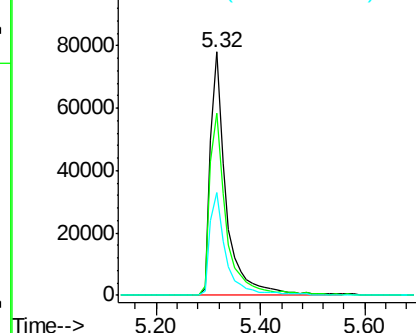



#7
 Phenol-d6
 Concen: 35.31 ng
 RT: 7.58 min Scan# 568
 Delta R.T. -0.07 min
 Lab File: BF081705.D
 Acq: 18 Sep 2015 19:55

Tgt Ion: 99 Resp: 134385
 Ion Ratio Lower Upper
 99 100
 42 26.7 13.7 20.5#
 71 41.4 14.2 21.2#

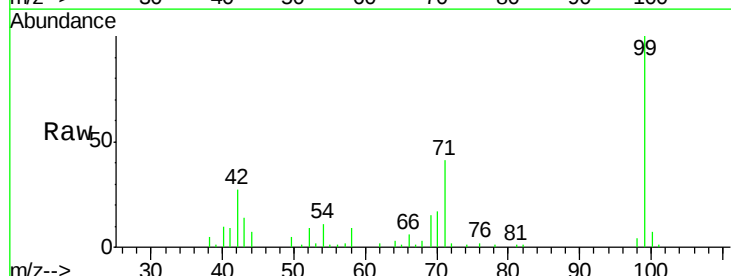

Abundance Ion 99.00 (98.70 to 99.70): BF0
 Ion 42.00 (41.70 to 42.70): BF0
 Ion 71.00 (70.70 to 71.70): BF0

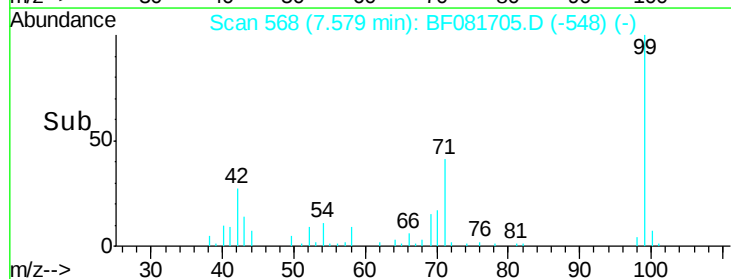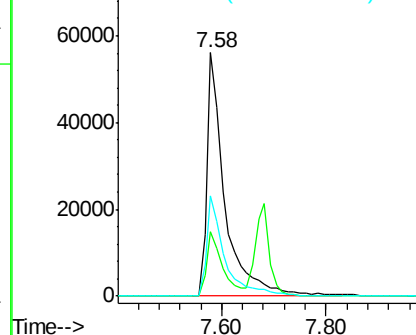

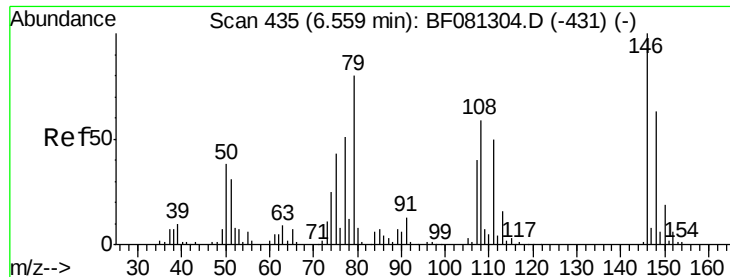

#15

Benzyl Alcohol

Concen: 2.12 ng

RT: 8.49 min Scan# 648

Delta R.T. -0.17 min

Lab File: BF081705.D

Acq: 18 Sep 2015 19:55

Instrument :

BNA_F

ClientSampleId :

MW-11-9-15-15


Tgt Ion: 79 Resp: 6623

Ion Ratio Lower Upper

79 100

108 27.8 88.6 132.8#




77 105.4 47.0 70.4#

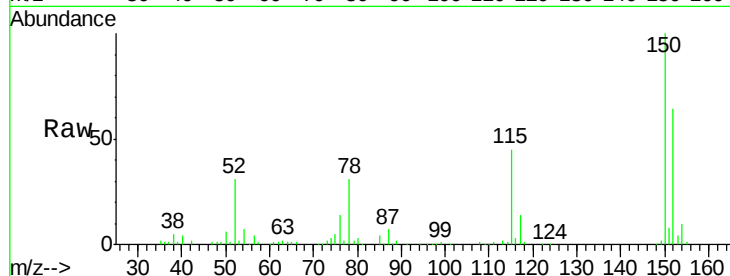

Abundance Ion 79.00 (78.70 to 79.70): BF0

Ion 108.00 (107.70 to 108.70): BF0

Ion 77.00 (76.70 to 77.70): BF0

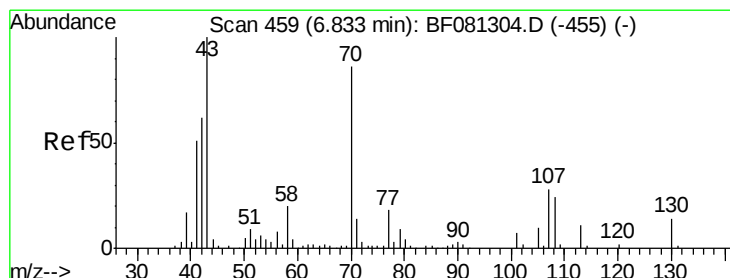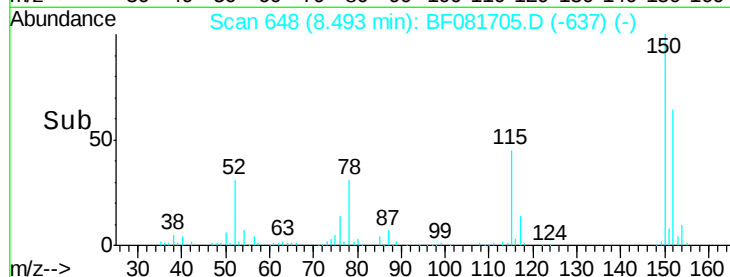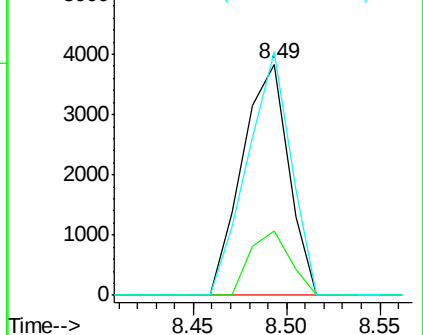

#19

n-Nitroso-di-n-propylamine

Concen: 20.28 ng

RT: 9.46 min Scan# 733

Delta R.T. 0.17 min

Lab File: BF081705.D

Acq: 18 Sep 2015 19:55

Tgt Ion: 70 Resp: 52519


Ion Ratio Lower Upper

70 100

42 61.6 63.8 95.6#

101 0.0 9.2 13.8#

130 1.8 27.3 40.9#


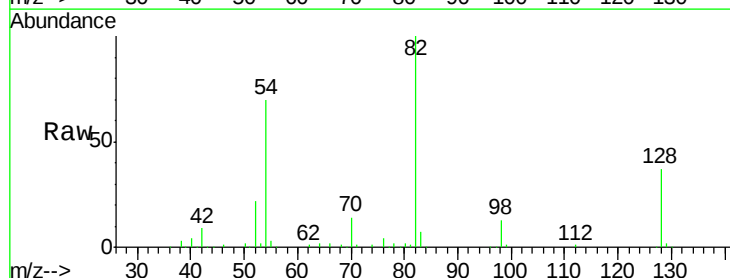



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

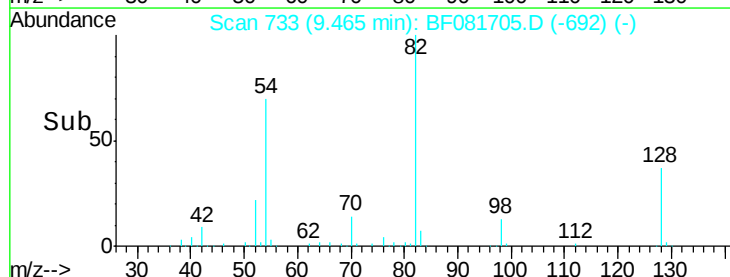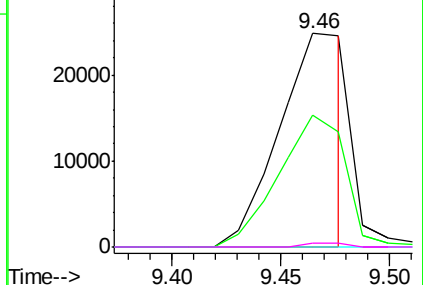



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.06 min Scan# 873

Delta R.T. -0.06 min

Lab File: BF081705.D

Acq: 18 Sep 2015 19:55


Instrument :

BNA_F

ClientSampleId :

MW-11-9-15-15

Tgt Ion:	136	Resp:	171702
Ion	Ratio	Lower	Upper
136	100		
137	10.5	9.0	13.6
54	11.1	8.2	12.2
68	4.7	5.8	8.6#



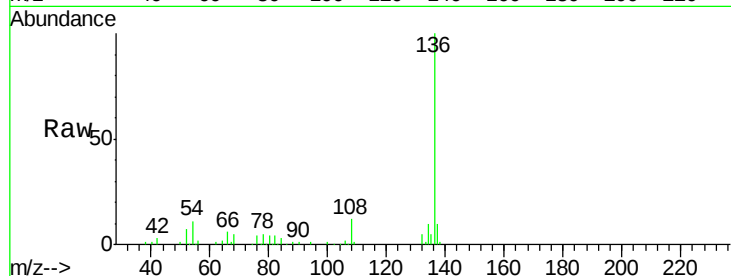


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

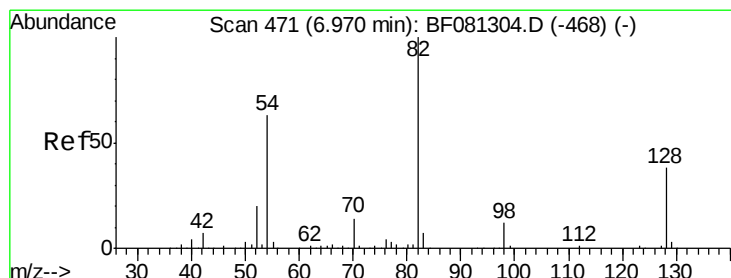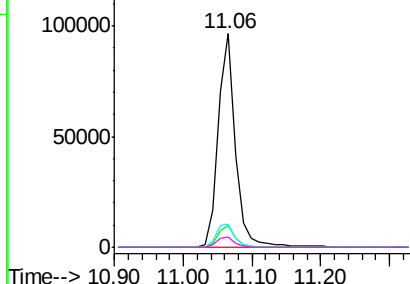

#23

Nitrobenzene-d5

Concen: 113.81 ng


RT: 9.46 min Scan# 733

Delta R.T. -0.07 min

Lab File: BF081705.D

Acq: 18 Sep 2015 19:55



Tgt Ion:	82	Resp:	405043
Ion	Ratio	Lower	Upper
82	100		
128	36.9	51.0	76.6#
54	69.8	47.5	71.3

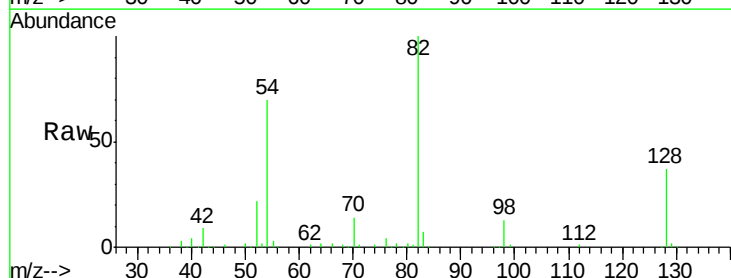


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

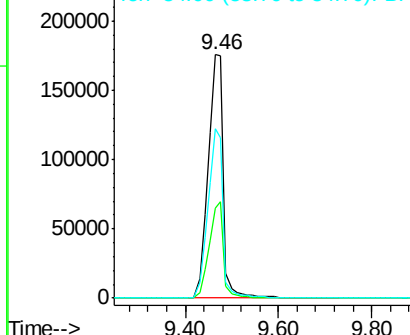



#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 15.19 min Scan# 1234

Delta R.T. -0.07 min

Lab File: BF081705.D

Acq: 18 Sep 2015 19:55

Instrument :

BNA_F

ClientSampleId :

MW-11-9-15-15


Tgt Ion:164 Resp: 84133

Ion Ratio Lower Upper

164 100

162 103.3 75.2 112.8




160 46.1 31.5 47.3

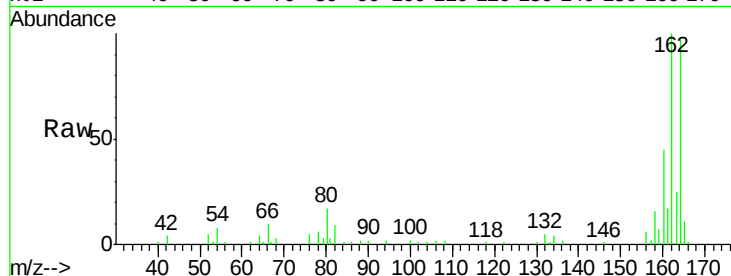

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

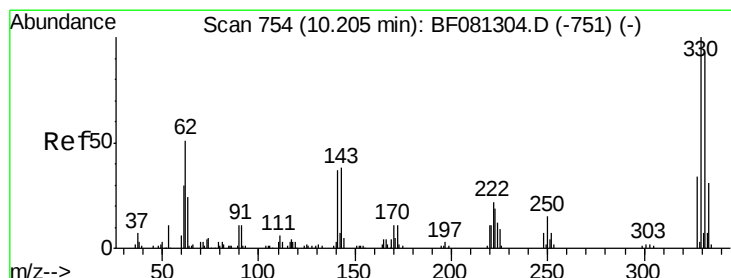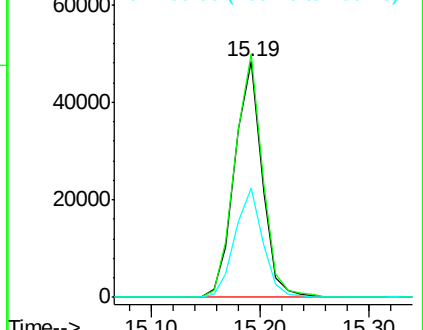

#41

2,4,6-Tribromophenol

Concen: 171.02 ng

RT: 17.10 min Scan# 1401

Delta R.T. -0.07 min

Lab File: BF081705.D

Acq: 18 Sep 2015 19:55


Tgt Ion:330 Resp: 128118

Ion Ratio Lower Upper

330 100

332 97.9 76.6 114.8



141 47.7 29.7 44.5#

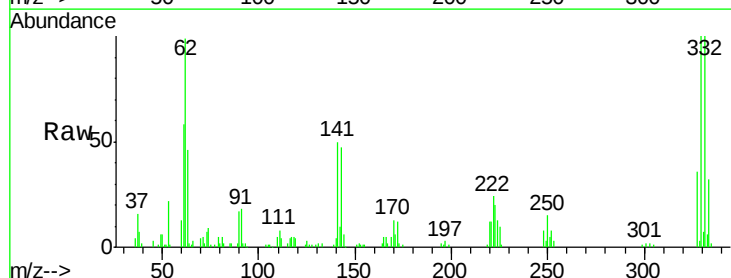


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




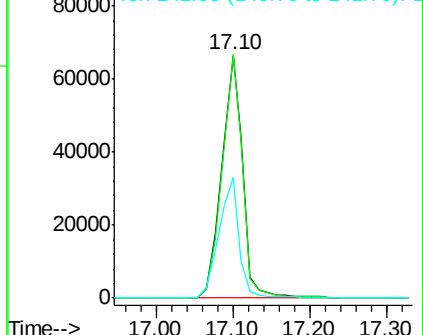


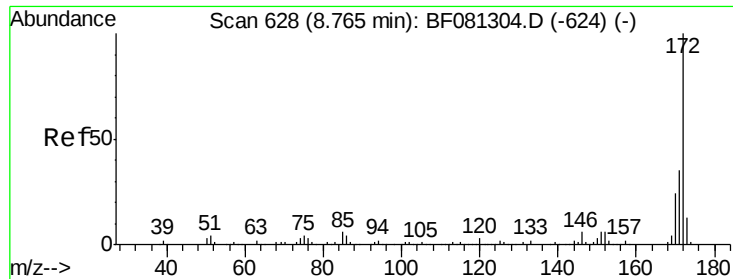

#44
 2-Fluorobiphenyl
 Concen: 108.89 ng
 RT: 13.72 min Scan# 1105
 Delta R.T. -0.06 min
 Lab File: BF081705.D
 Acq: 18 Sep 2015 19:55




Instrument :
 BNA_F
 ClientSampleId :
 MW-11-9-15-15


Tgt Ion:172 Resp: 714877
 Ion Ratio Lower Upper
 172 100
 171 34.3 26.1 39.1
 170 23.7 17.4 26.2

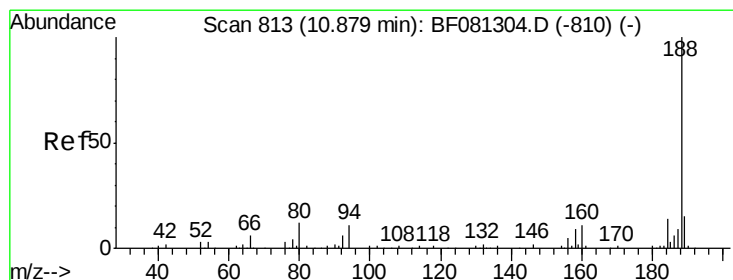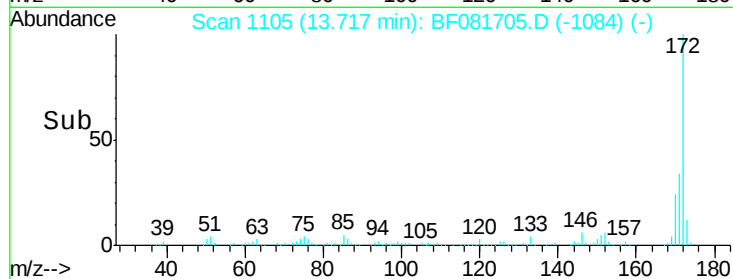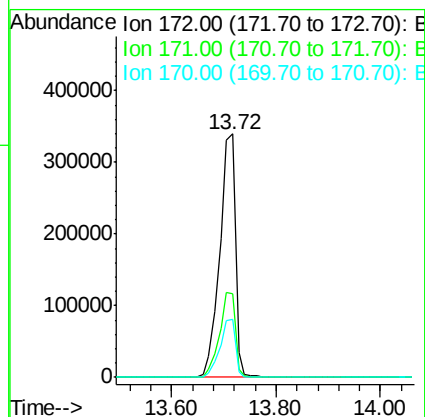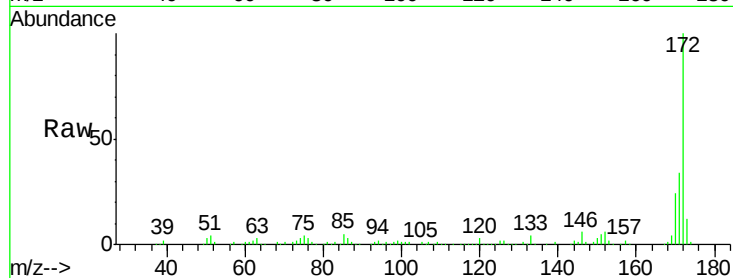

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 18.70 min Scan# 1541
 Delta R.T. -0.06 min
 Lab File: BF081705.D
 Acq: 18 Sep 2015 19:55

Tgt Ion:188 Resp: 174670
 Ion Ratio Lower Upper
 188 100
 94 7.3 11.1 16.7#
 80 7.9 11.0 16.4#

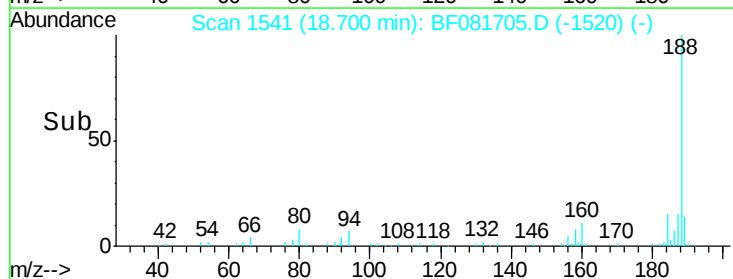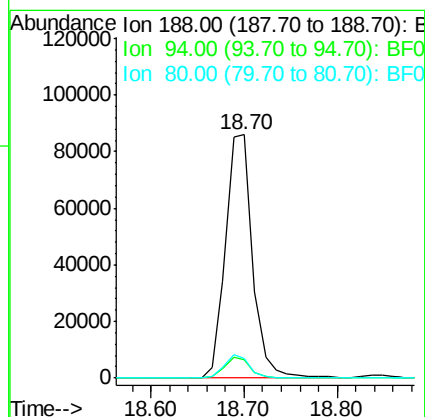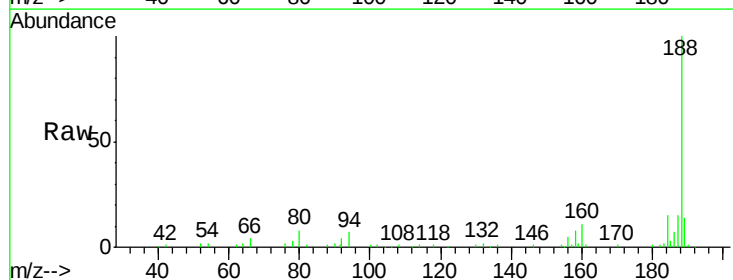



#75

Chrysene-d12

Concen: 20.00 ng

RT: 23.34 min Scan# 1947

Delta R.T. -0.04 min

Lab File: BF081705.D

Acq: 18 Sep 2015 19:55

Instrument :

BNA_F

ClientSampleId :

MW-11-9-15-15


Tgt Ion:240 Resp: 137655

Ion Ratio Lower Upper

240 100

120 11.4 16.2 24.2#




236 25.5 18.4 27.6

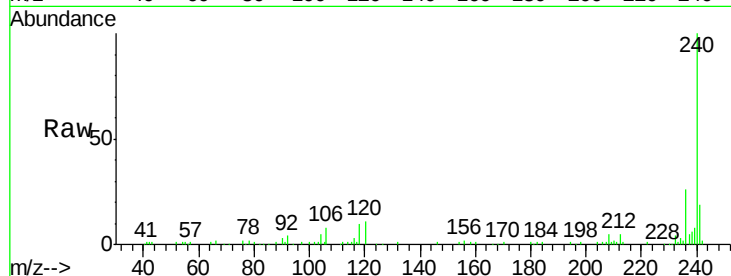

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

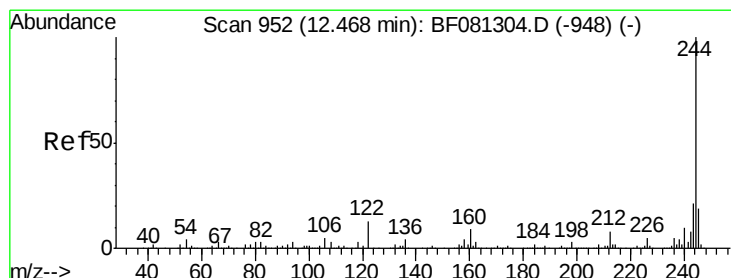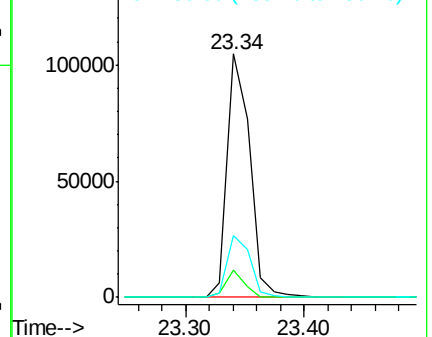

#78

Terphenyl-d14

Concen: 101.12 ng

RT: 22.07 min Scan# 1836

Delta R.T. -0.04 min

Lab File: BF081705.D

Acq: 18 Sep 2015 19:55


Tgt Ion:244 Resp: 597960

Ion Ratio Lower Upper

244 100

212 7.7 4.3 6.5#



122 12.6 17.4 26.2#

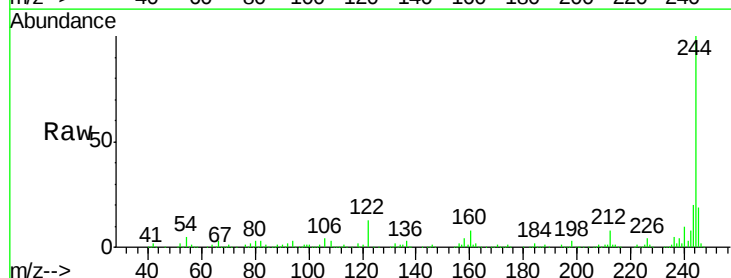


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

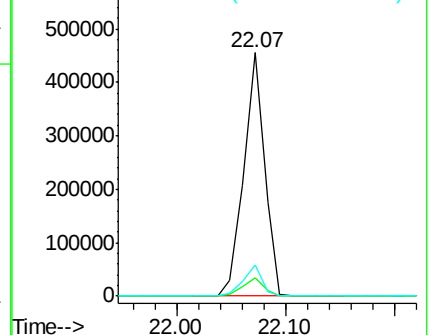


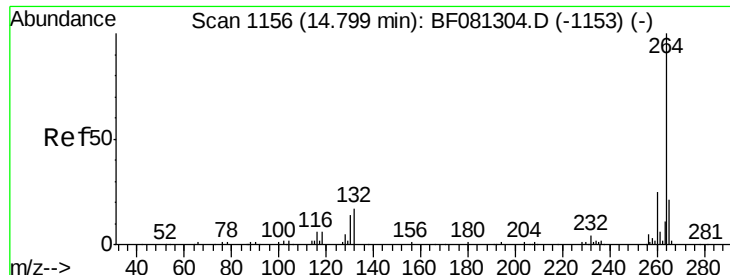

#86
Perylene-d12
Concen: 20.00 ng
RT: 24.78 min Scan# 2073
Delta R.T. -0.03 min
Lab File: BF081705.D
Acq: 18 Sep 2015 19:55

Instrument :
BNA_F
ClientSampleId :
MW-11-9-15-15

Tgt Ion: 264 Resp: 96336
Ion Ratio Lower Upper
264 100
260 23.6 16.7 25.1
265 20.5 17.2 25.8

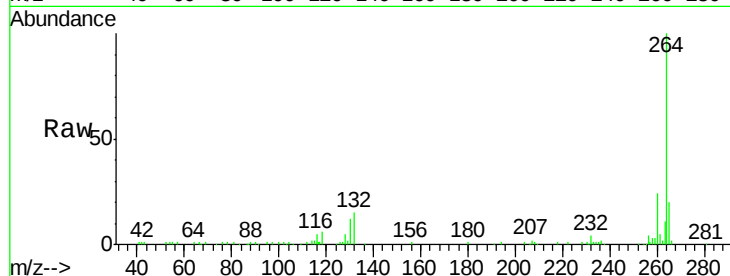

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

