
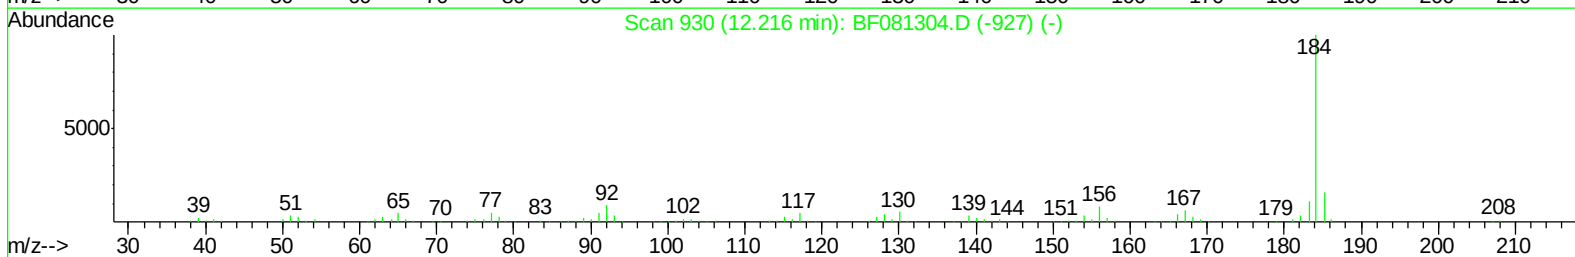
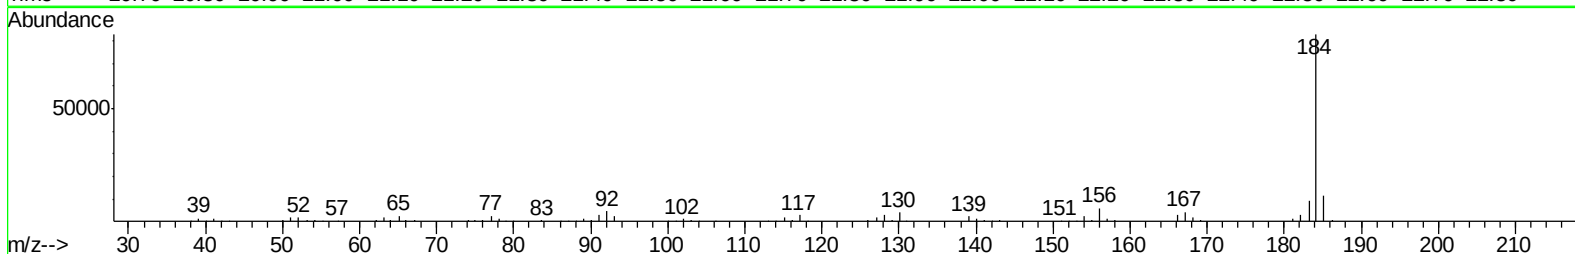


Data Path : Z:\HPCHEM1\BNA F\Data\BF091815\
Data File : BF081693.D
Acq On : 18 Sep 2015 11:45
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 02:39:37 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 15 14:03:59 2015
Response via : Initial Calibration

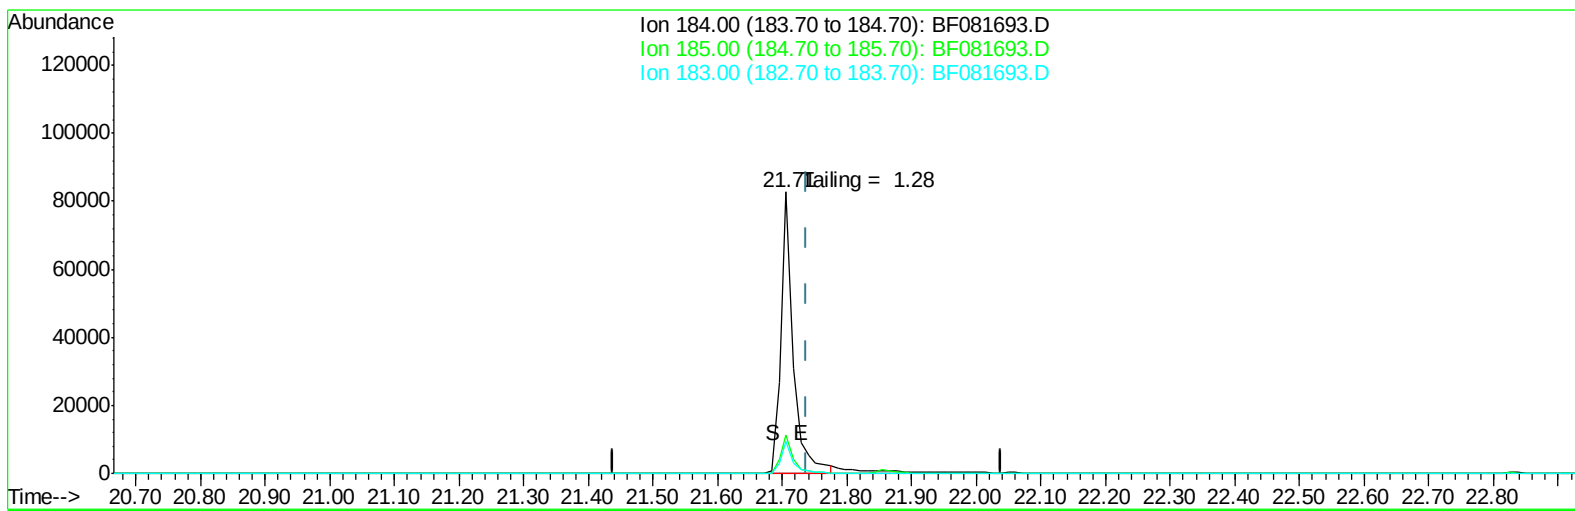

TIC: BF081693.D

(76) Benzidine




21.706min (-0.033) 0.00ng

response 119613

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.78
183.00	9.50	11.19
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF091815\
Data File : BF081693.D
Acq On : 18 Sep 2015 11:45
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 02:39:37 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 15 14:03:59 2015
Response via : Initial Calibration

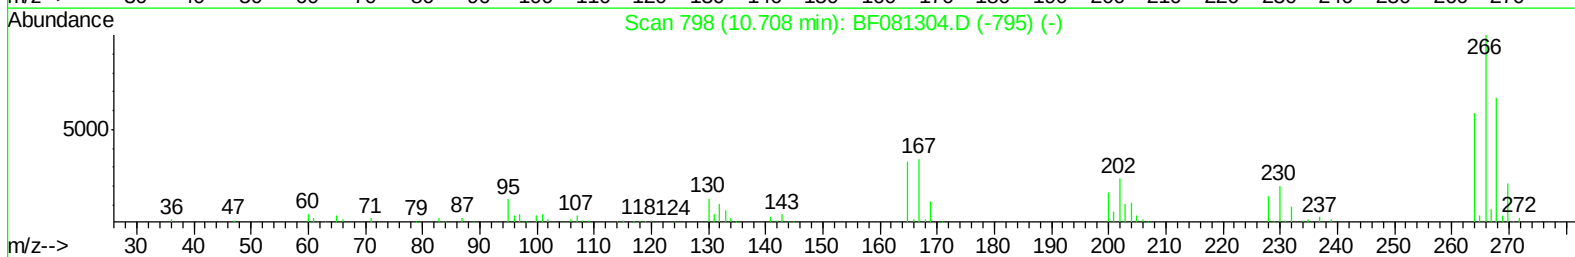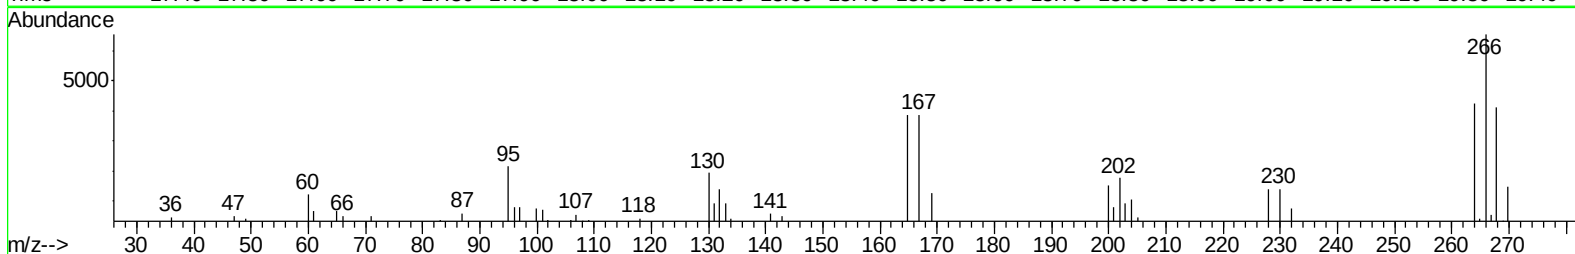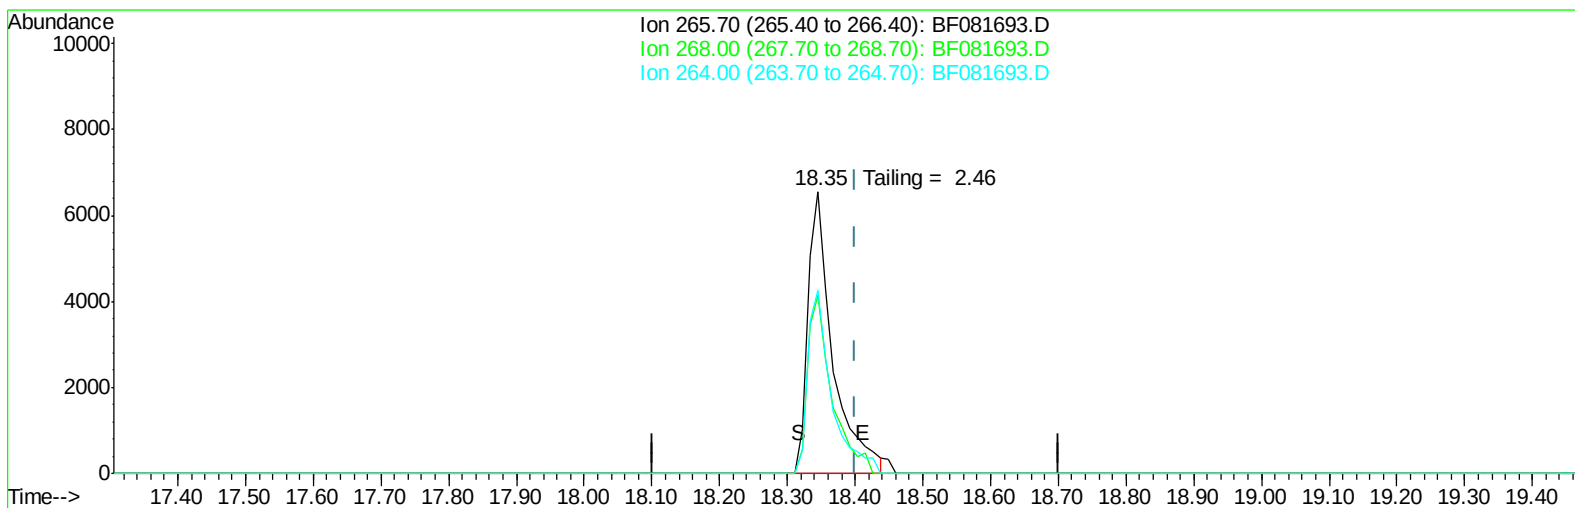

TIC: BF081693.D

(69) Pentachlorophenol (C)

18.346min (-0.056) 0.00ng

response 16818

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.21
264.00	62.70	64.86
0.00	0.00	0.00