


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091815\
 Data File : BF081693.D
 Acq On : 18 Sep 2015 11:45
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 15 14:03:59 2015

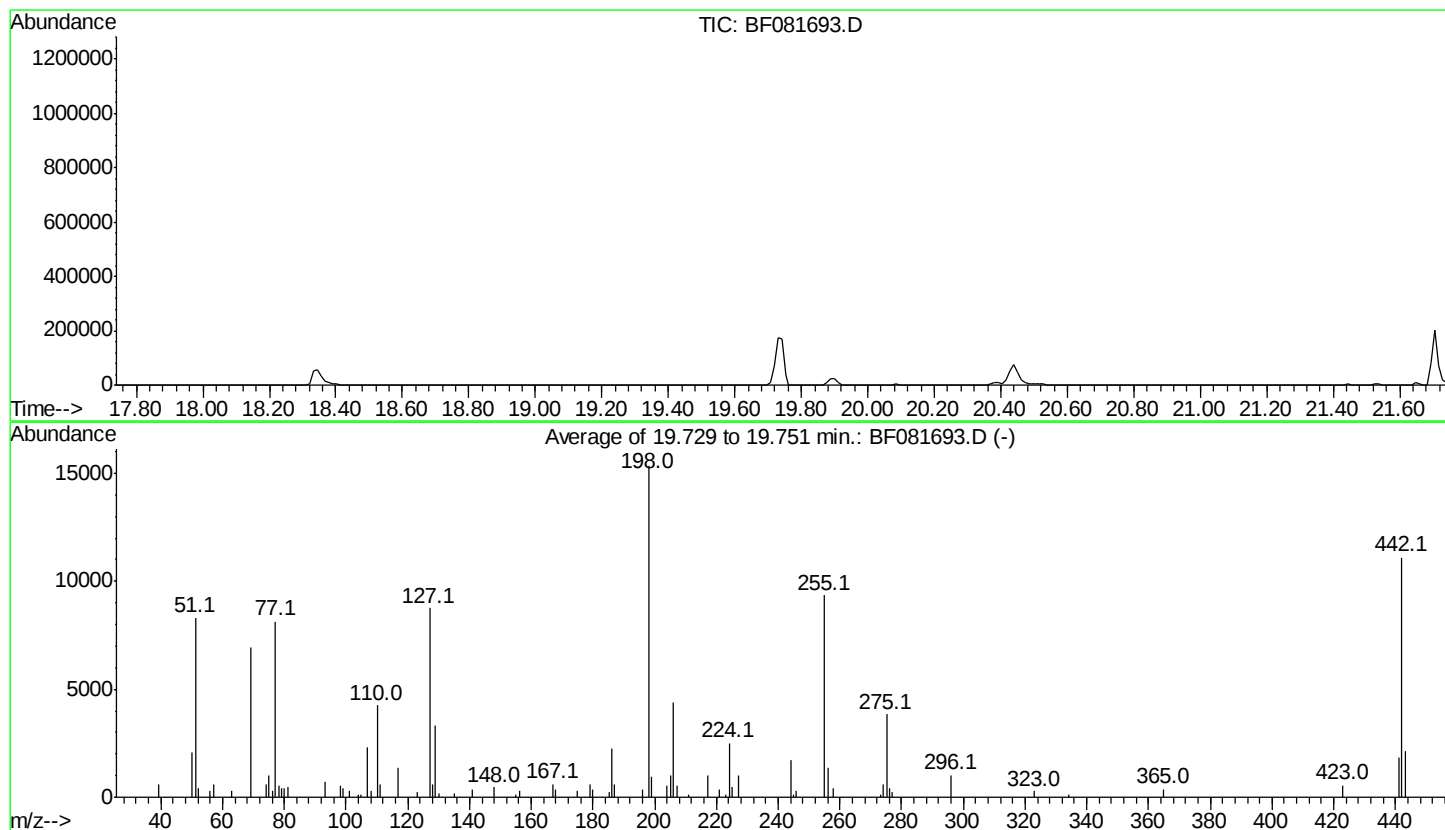

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.1	8303	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.3	6950	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.1	8761	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	15355	PASS
199	198	5	9	6.1	936	PASS
275	198	10	60	25.0	3833	PASS
365	198	1	100	2.4	372	PASS
441	442	0.01	24	16.8	1867	PASS
442	198	50	100	72.3	11094	PASS
443	442	15	24	19.3	2138	PASS