

Data Path : Z:\HPCHEM1\BNA F\DATA\BF091817\
 Data File : BF098627.D
 Acq On : 19 Sep 2017 3:37
 Operator : SJ/JU
 Sample : I5262-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Sep 19 05:43:28 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 18 13:37:24 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.63	152	110709	20.00	ng	0.00
21) Naphthalene-d8	7.92	136	480218	20.00	ng	0.00
38) Acenaphthene-d10	9.67	164	184079	20.00	ng	0.00
63) Phenanthrene-d10	11.15	188	357059	20.00	ng	0.00
75) Chrysene-d12	13.78	240	236891	20.00	ng	0.00
86) Perylene-d12	15.18	264	231443	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.24	112	295166	39.42	ng	0.00
7) Phenol-d6	6.29	99	256736	27.00	ng	0.00
23) Nitrobenzene-d5	7.20	82	650980	75.57	ng	0.00
41) 2,4,6-Tribromophenol	10.46	330	110775	90.17	ng	0.00
44) 2-Fluorobiphenyl	9.00	172	1231134	113.36	ng	0.00
78) Terphenyl-d14	12.73	244	886942	80.81	ng	0.00
Target Compounds						
9) Benzaldehyde	6.40	77	12606	2.028	ng	# 68
19) n-Nitroso-di-n-propylamine	7.20	70	87574	14.644	ng	# 79
25) Isophorone	7.20	82	650974	37.352	ng	# 67
49) Dimethylphthalate	9.39	163	44831	3.146	ng	# 97
50) 2,6-Dinitrotoluene	9.67	165	22828	7.799	ng	# 34
56) 2,4-Dinitrotoluene	9.67	165	22828	6.415	ng	# 33
64) 4,6-Dinitro-2-methylphenol	10.46	198	250	5.067	ng	# 1
66) 4-Bromophenyl-phenylether	10.46	248	8369	2.470	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF091817\
Data File : BF098627.D
Acq On : 19 Sep 2017 3:37
Operator : SJ/JU
Sample : I5262-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Sep 19 05:43:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 18 13:37:24 2017
Response via : Initial Calibration

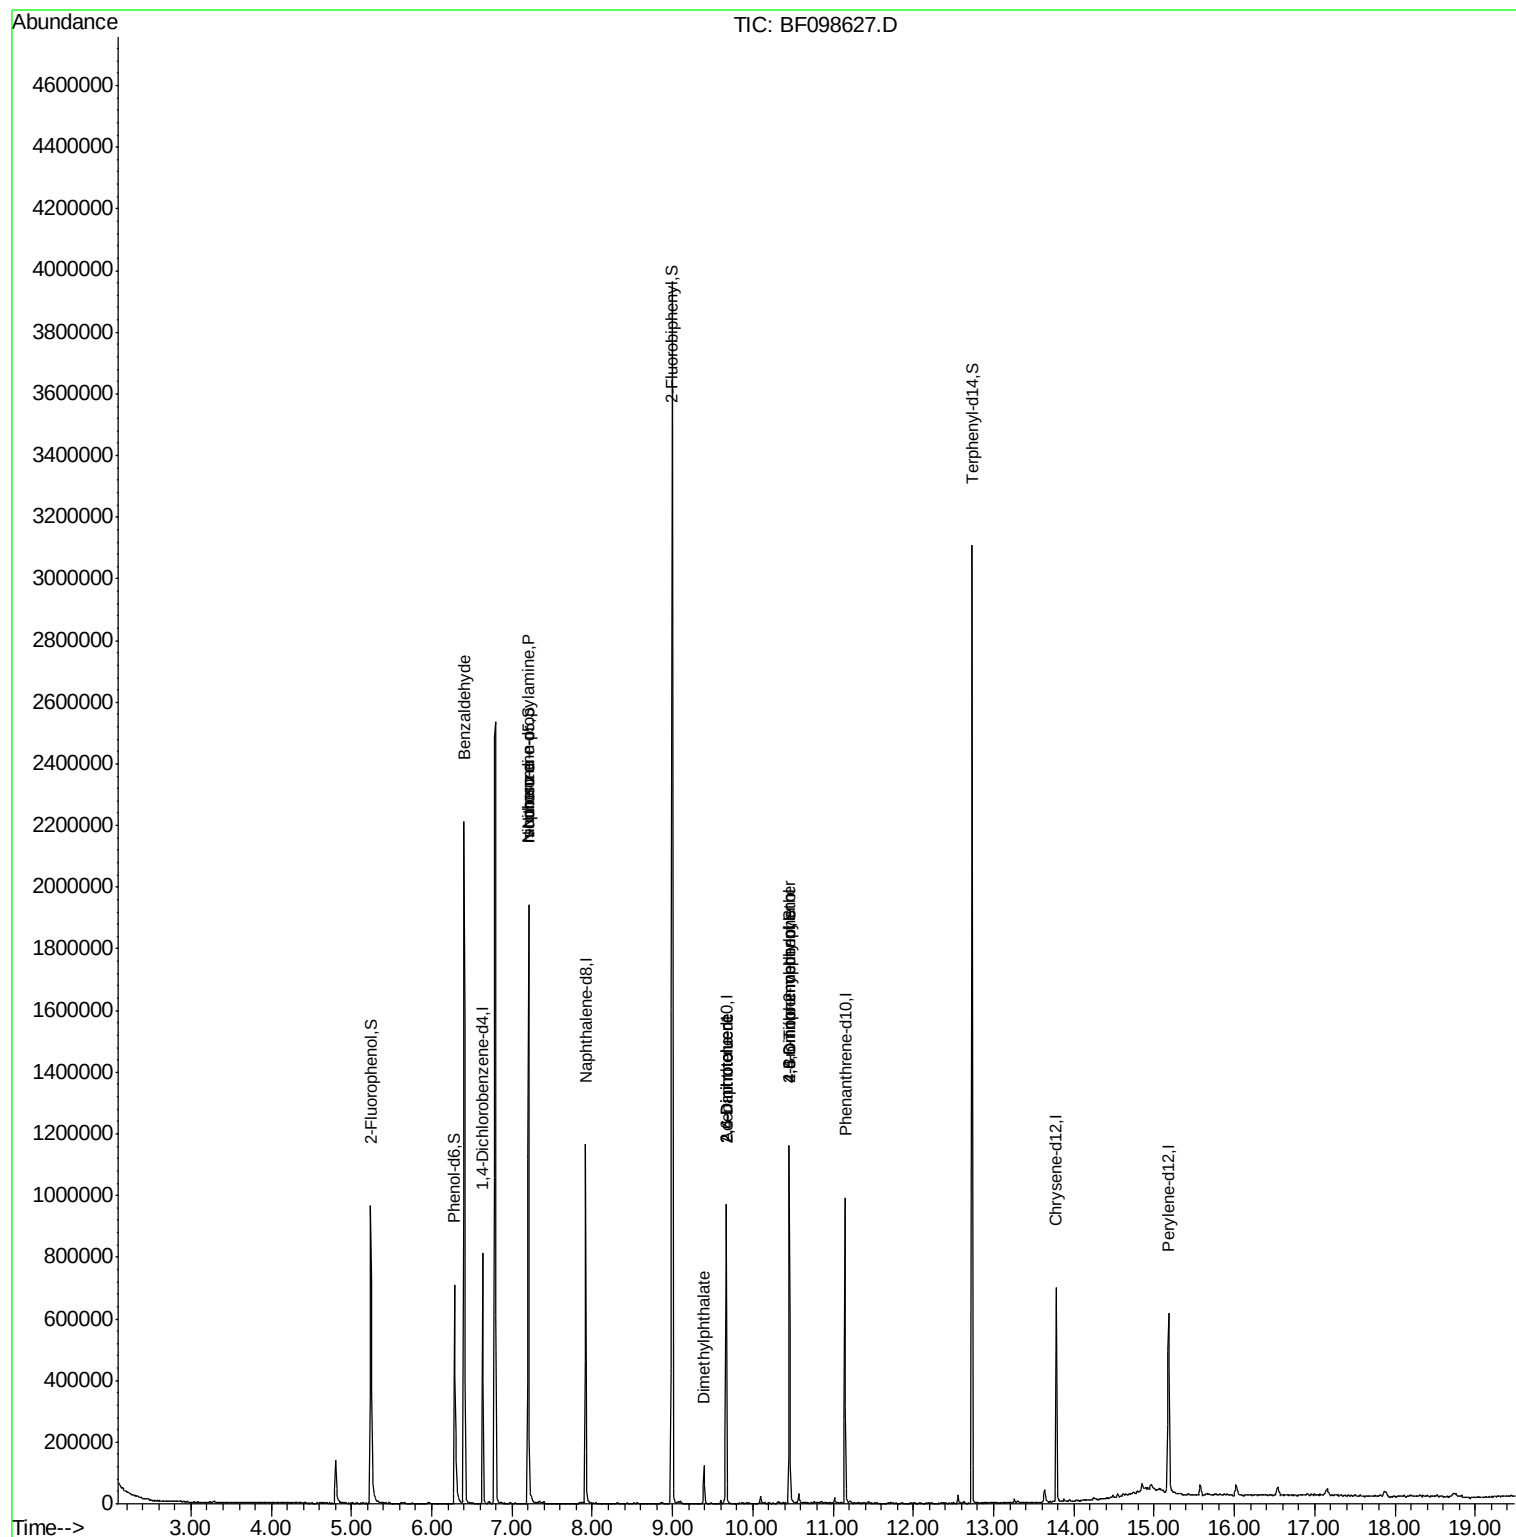




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.63 min Scan# 773
Delta R.T. 0.00 min
Lab File: BF098627.D
Acq: 19 Sep 2017 3:37

Instrument :
BNA_F
ClientSampled :

Tot Ion:152 Resp: 110709
Ion Ratio Lower Upper
152 100
150 159.5 126.2 189.2
115 65.8 52.2 78.2

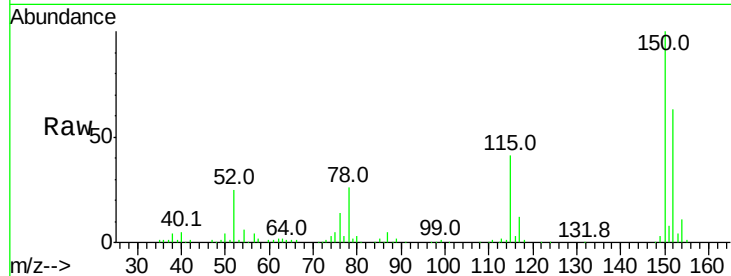


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

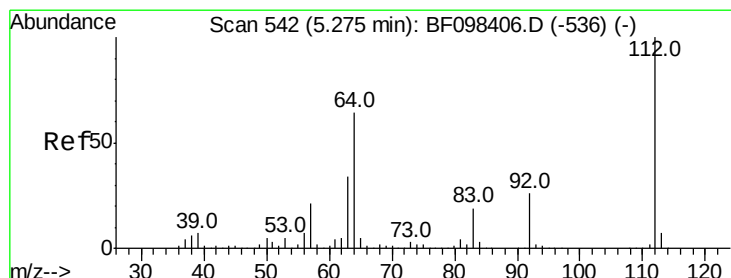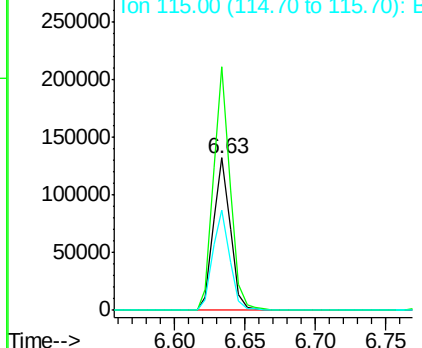



#5


2-Fluorophenol
Concen: 39.420 ng
RT: 5.24 min Scan# 536
Delta R.T. 0.00 min
Lab File: BF098627.D
Acq: 19 Sep 2017 3:37

Tgt Ion:112 Resp: 295166
Ion Ratio Lower Upper
112 100
64 65.8 46.0 69.0
63 33.4 23.4 35.0

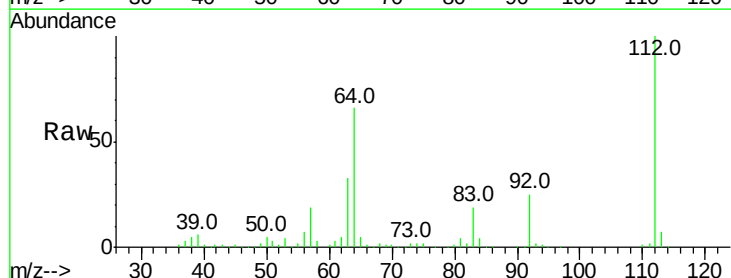

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

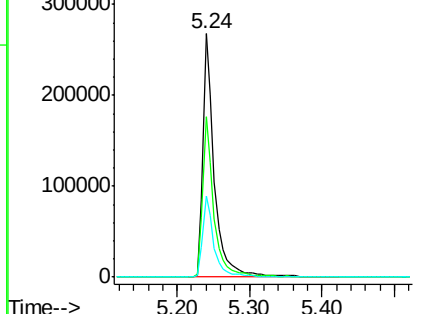

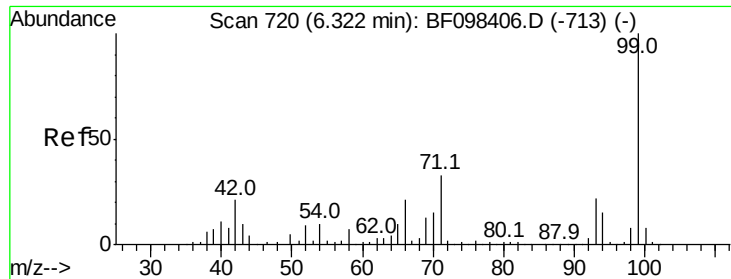

#7

Phenol-d6

Concen: 27.005 ng

RT: 6.29 min Scan# 714

Delta R.T. -0.01 min

Lab File: BF098627.D

Acq: 19 Sep 2017 3:37

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 256736

Ion Ratio Lower Upper

99 100

42 19.8 13.5 20.3




71 34.8 24.5 36.7

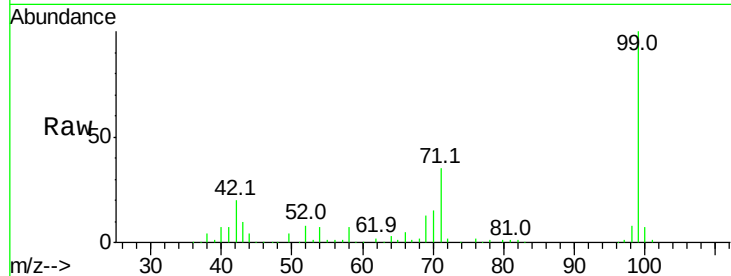

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

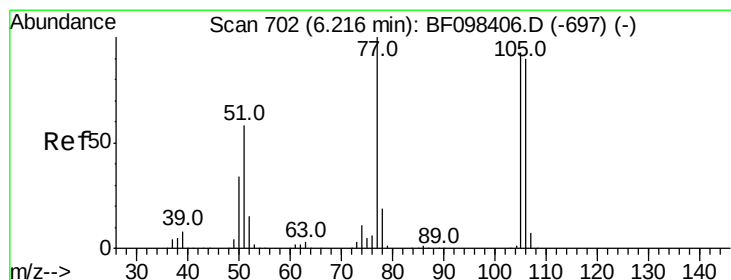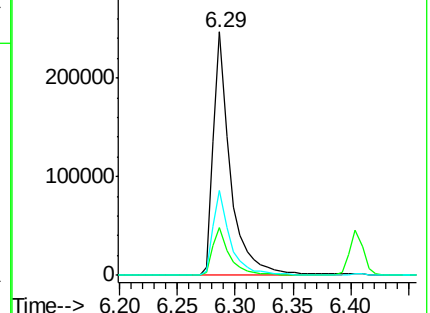

#9

Benzaldehyde

Concen: 2.028 ng

RT: 6.40 min Scan# 734

Delta R.T. 0.22 min

Lab File: BF098627.D

Acq: 19 Sep 2017 3:37


Tgt Ion: 77 Resp: 12606

Ion Ratio Lower Upper

77 100

105 67.4 83.8 123.8#



106 70.8 79.1 119.1#

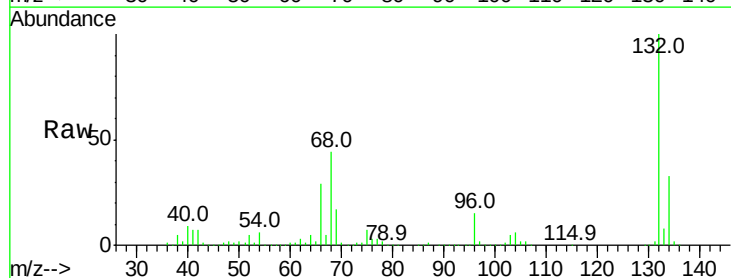


Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E

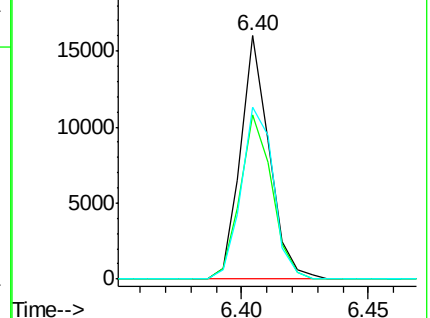

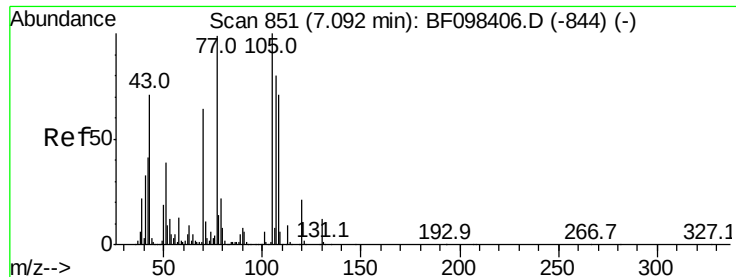

#19

n-Nitroso-di-n-propylamine

Concen: 14.644 ng

RT: 7.20 min Scan# 870

Delta R.T. 0.15 min

Lab File: BF098627.D





Acq: 19 Sep 2017 3:37

Instrument :

BNA_F

ClientSampleId :

Tot Ion:	70	Resp:	87574
Ion	Ratio	Lower	Upper
70	100		
42	48.4	47.2	70.8
101	0.0	7.2	10.8#
130	1.9	15.9	23.9#

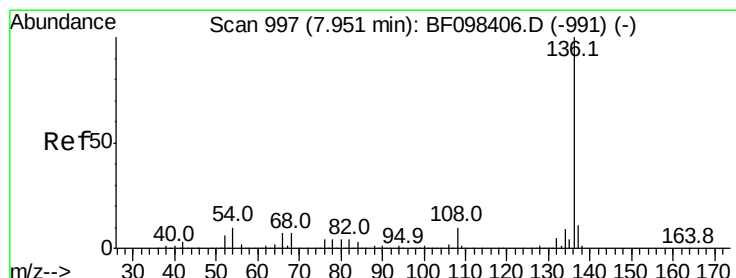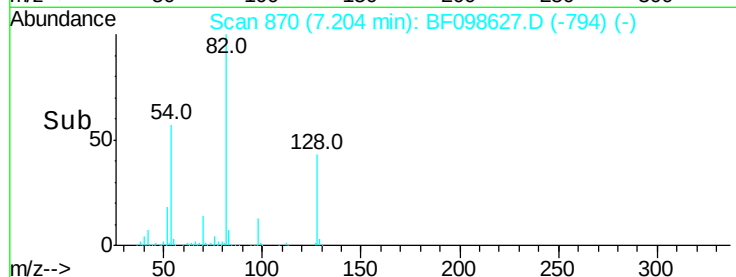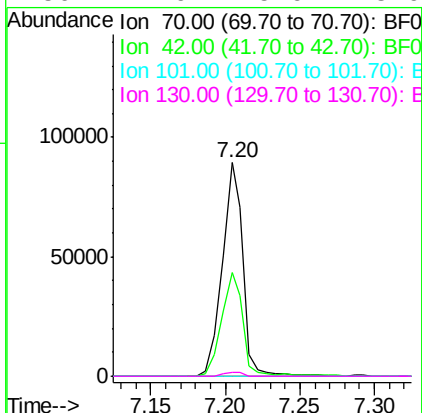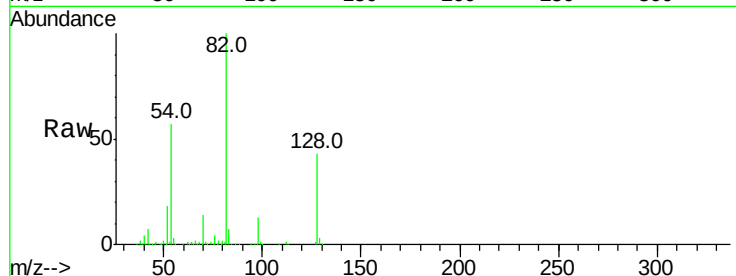

#21

Naphthalene-d8

Concen: 20.000 ng




RT: 7.92 min Scan# 991


Delta R.T. -0.01 min

Lab File: BF098627.D

Acq: 19 Sep 2017 3:37

Tgt Ion:	136	Resp:	480218
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.5	12.7
54	9.1	4.9	7.3#
68	5.6	4.1	6.1

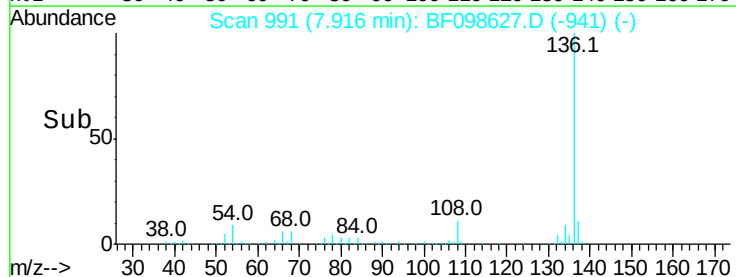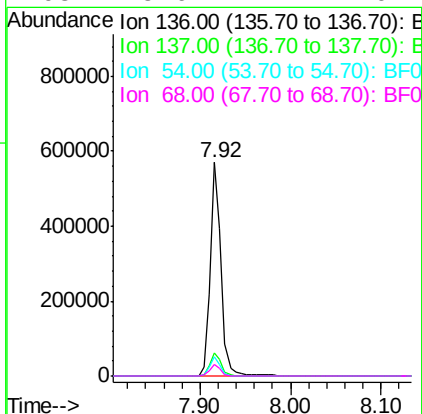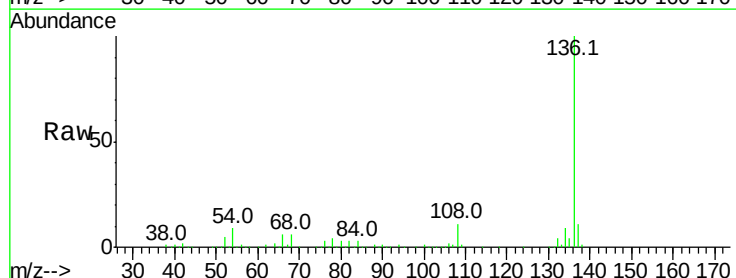

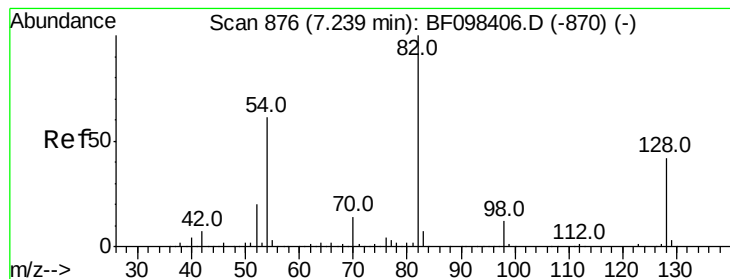

#23

Nitrobenzene-d5

Concen: 75.574 ng

RT: 7.20 min Scan# 870

Delta R.T. -0.01 min

Lab File: BF098627.D

Acq: 19 Sep 2017 3:37

Instrument :

BNA_F

ClientSampled :


Tot Ion: 82 Resp: 650980

Ion Ratio Lower Upper

82 100

128 42.7 34.0 51.0




54 56.6 42.2 63.2

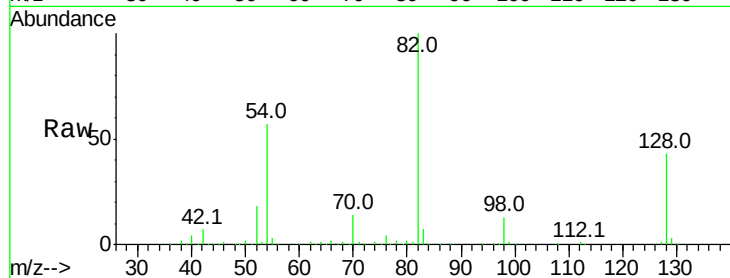

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): BF0

Ion 54.00 (53.70 to 54.70): BF0

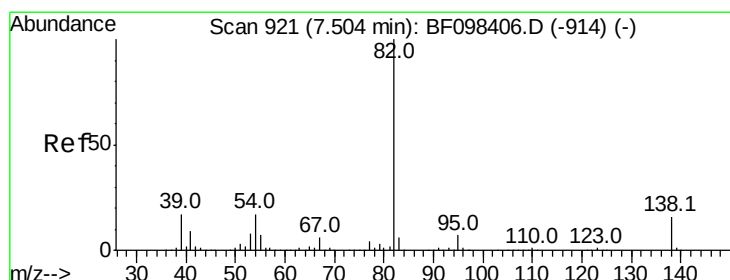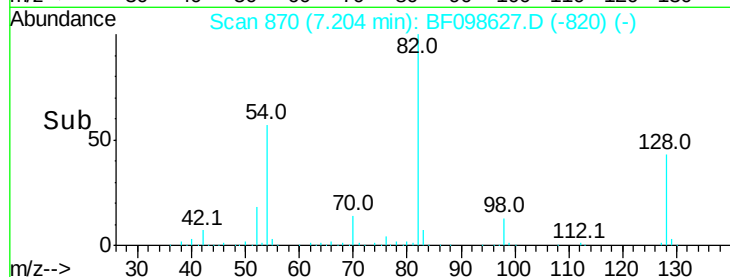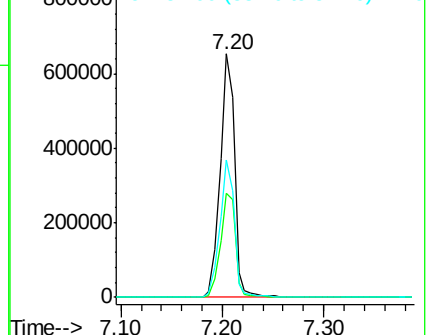

#25

Isophorone

Concen: 37.352 ng

RT: 7.20 min Scan# 870

Delta R.T. -0.26 min

Lab File: BF098627.D

Acq: 19 Sep 2017 3:37


Tgt Ion: 82 Resp: 650974

Ion Ratio Lower Upper

82 100

95 0.0 5.3 7.9#



138 0.0 13.1 19.7#

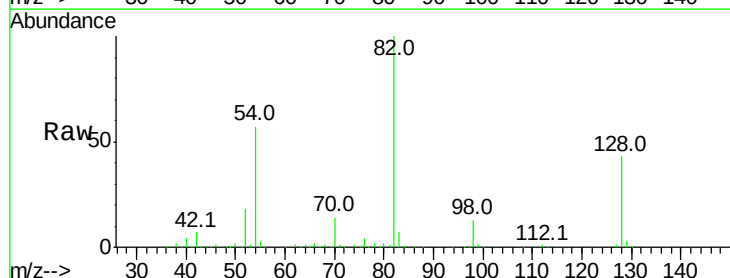


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 95.00 (94.70 to 95.70): BF0

Ion 138.00 (137.70 to 138.70): BF0



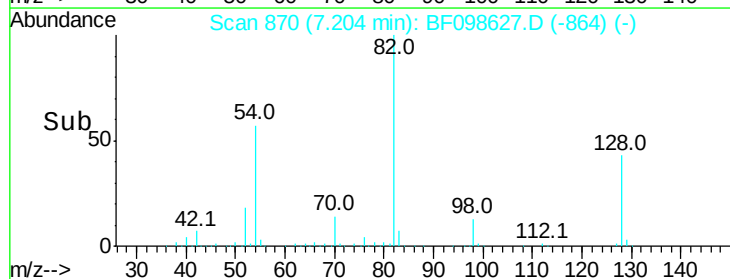
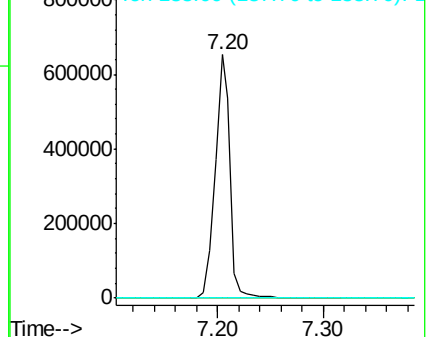


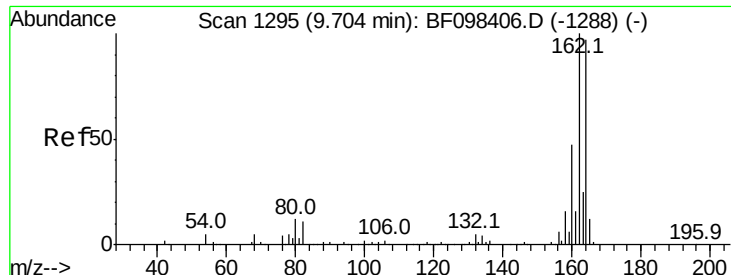

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.67 min Scan# 1289
 Delta R.T. 0.00 min
 Lab File: BF098627.D
 Acq: 19 Sep 2017 3:37




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
164	100		
162	104.7	82.6	123.8
160	47.2	36.2	54.2

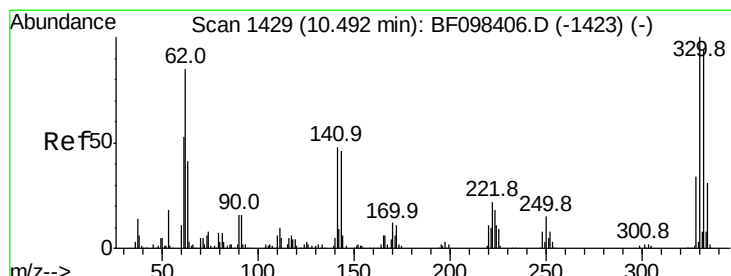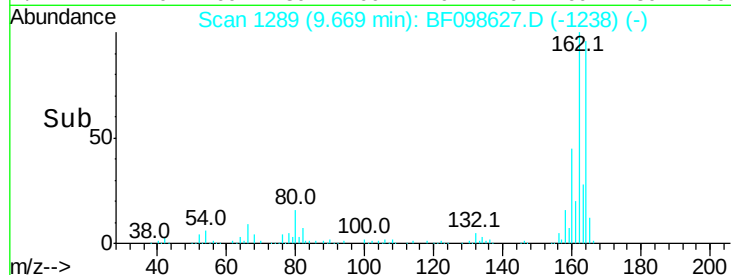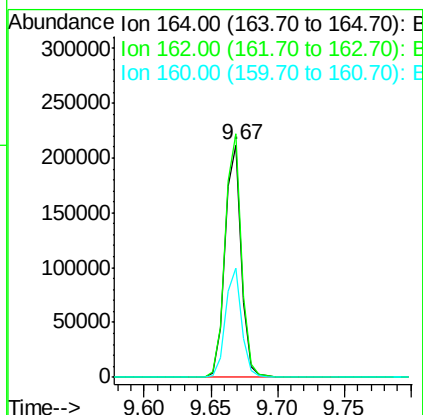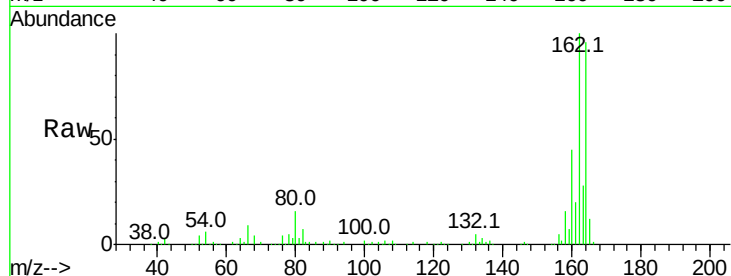

#41
 2,4,6-Tribromophenol
 Concen: 90.165 ng
 RT: 10.46 min Scan# 1423
 Delta R.T. -0.01 min
 Lab File: BF098627.D
 Acq: 19 Sep 2017 3:37

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.8	76.6	115.0
141	44.5	31.4	47.2


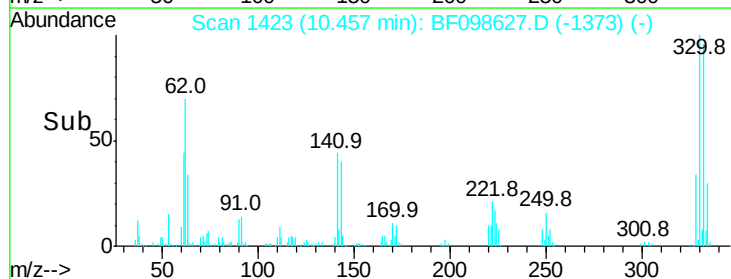
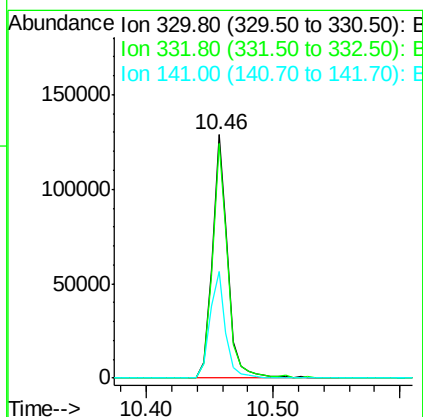
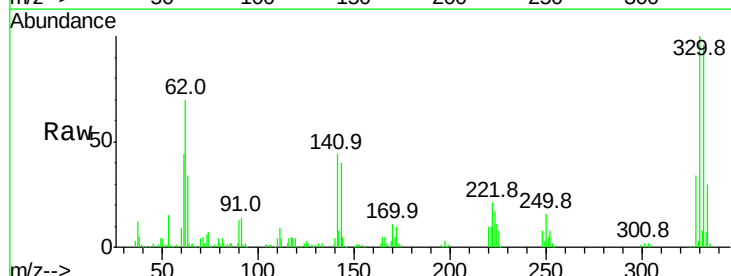


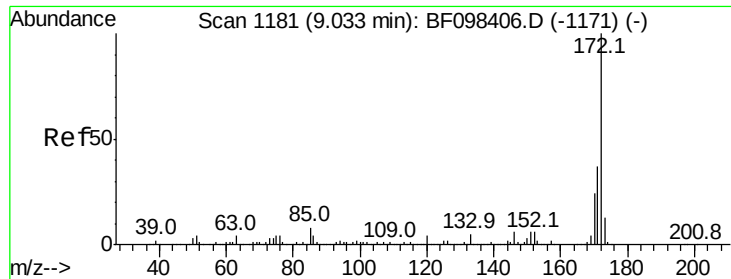

#44
2-Fluorobiphenyl
Concen: 113.357 ng
RT: 9.00 min Scan# 1175
Delta R.T. 0.00 min
Lab File: BF098627.D
Acq: 19 Sep 2017 3:37




Instrument :
BNA_F
ClientSampleId :


Tot Ion:172 Resp: 1231134
Ion Ratio Lower Upper
172 100
171 35.9 29.6 44.4
170 23.8 19.8 29.8

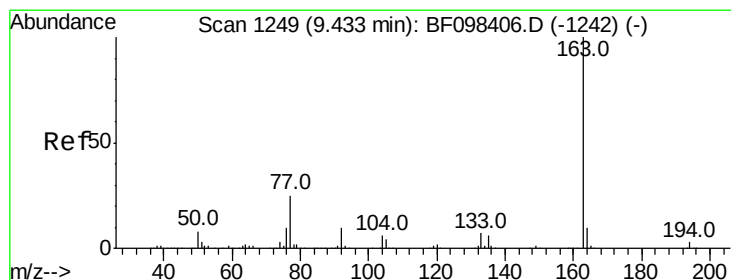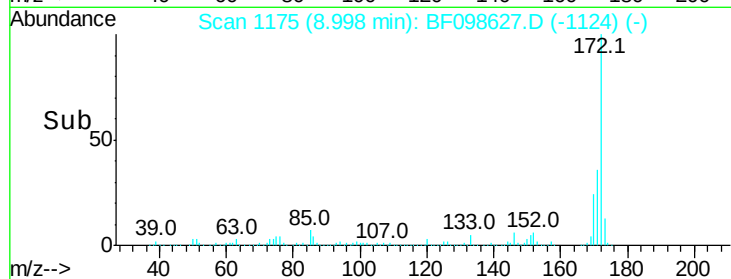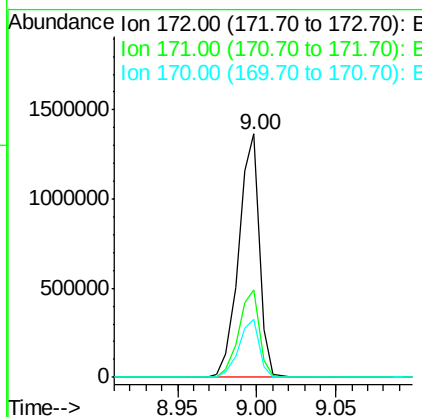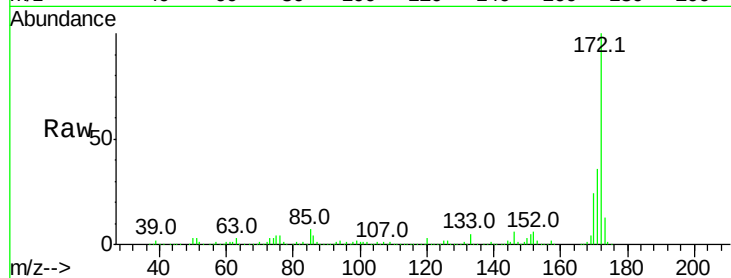

#49
Dimethylphthalate
Concen: 3.146 ng
RT: 9.39 min Scan# 1242
Delta R.T. -0.01 min
Lab File: BF098627.D
Acq: 19 Sep 2017 3:37

Tgt Ion:163 Resp: 44831
Ion Ratio Lower Upper
163 100
194 3.3 2.6 4.0
164 9.2 8.4 12.6

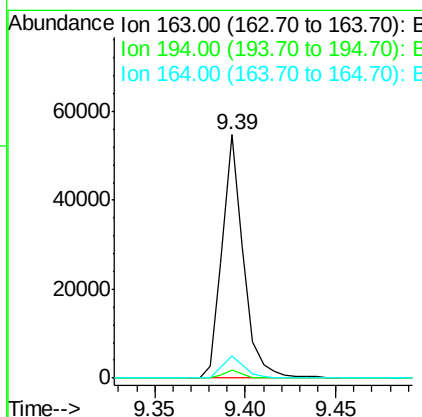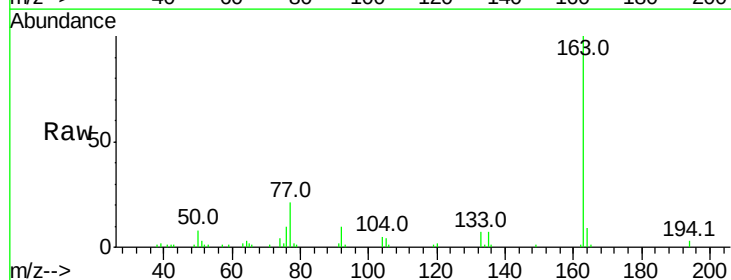


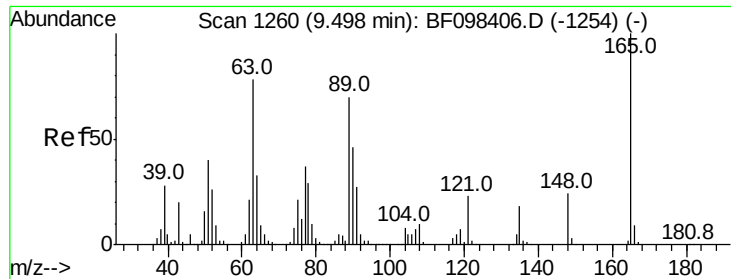

#50
 2,6-Dinitrotoluene
 Concen: 7.799 ng
 RT: 9.67 min Scan# 1289
 Delta R.T. 0.20 min
 Lab File: BF098627.D
 Acq: 19 Sep 2017 3:37

Instrument :
 BNA_F
 ClientSampleId :




Tot Ion	Ratio	Lower	Upper
165	100		
63	1.5	34.3	51.5#
89	1.8	37.1	55.7#

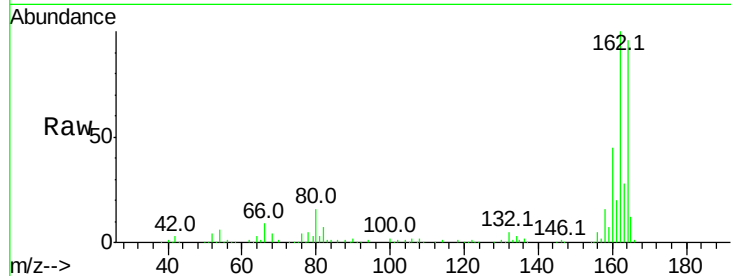

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

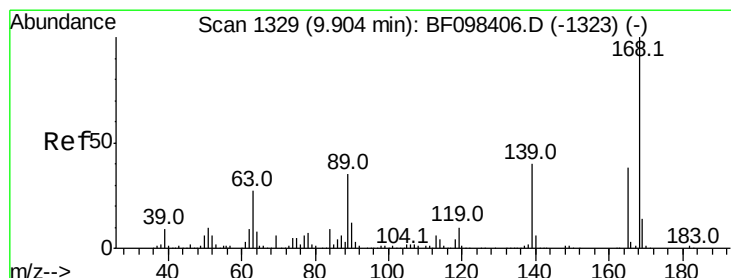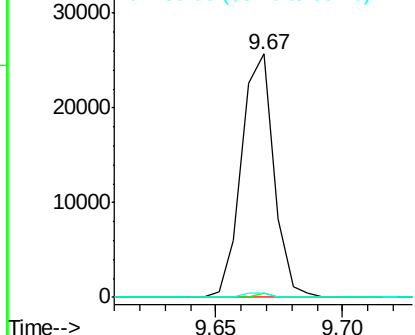

#56
 2,4-Dinitrotoluene
 Concen: 6.415 ng
 RT: 9.67 min Scan# 1289
 Delta R.T. -0.21 min
 Lab File: BF098627.D
 Acq: 19 Sep 2017 3:37




Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.5	25.4	38.0#
89	1.8	46.4	69.6#
182	0.0	1.8	2.6#


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E


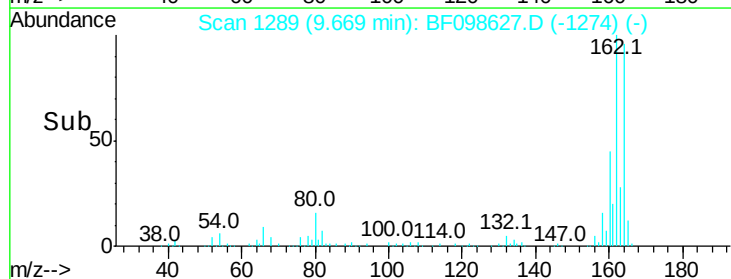
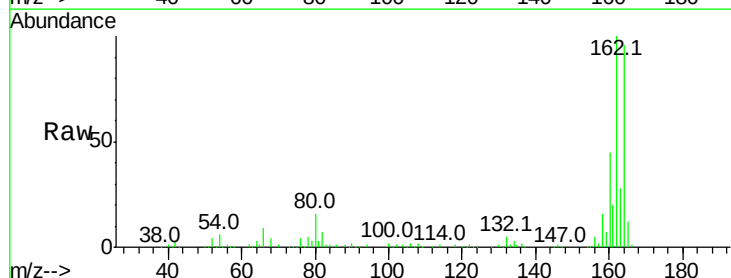
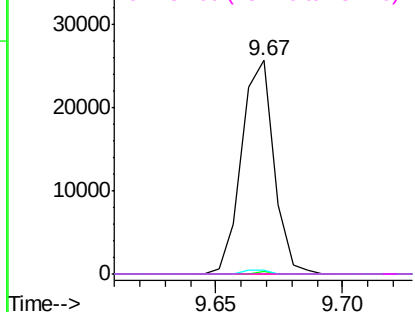




#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.15 min Scan# 1541
 Delta R.T. 0.00 min
 Lab File: BF098627.D
 Acq: 19 Sep 2017 3:37




Instrument :
 BNA_F
 ClientSampled :


Tot Ion:188 Resp: 357059
 Ion Ratio Lower Upper
 188 100
 94 8.8 9.4 14.2#
 80 9.7 10.2 15.2#

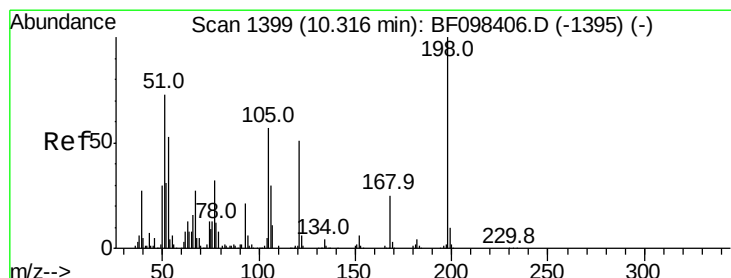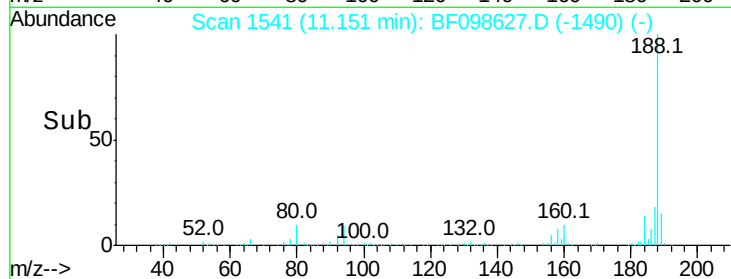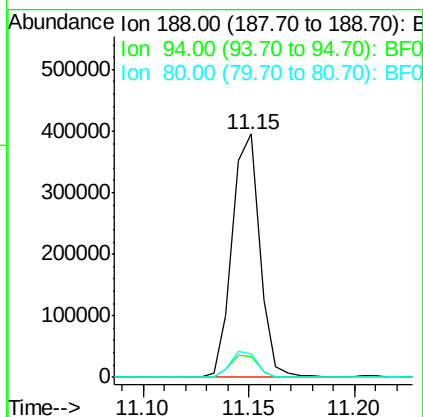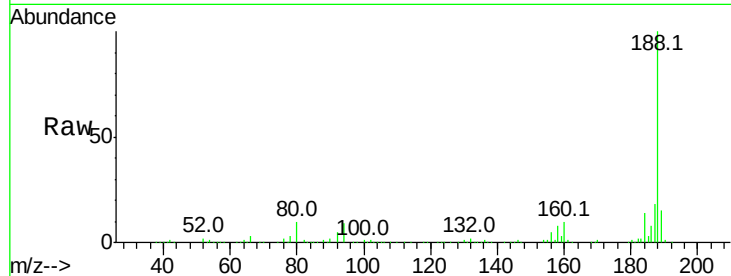

#64
 4,6-Dinitro-2-methylphenol
 Concen: 5.067 ng
 RT: 10.46 min Scan# 1423
 Delta R.T. 0.16 min
 Lab File: BF098627.D
 Acq: 19 Sep 2017 3:37

Tgt Ion:198 Resp: 250
 Ion Ratio Lower Upper
 198 100
 51 206.0 53.2 93.2#
 105 218.2 45.8 85.8#

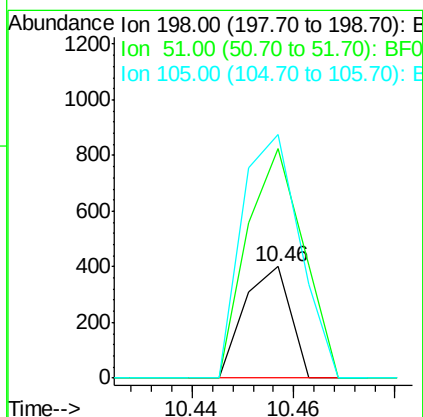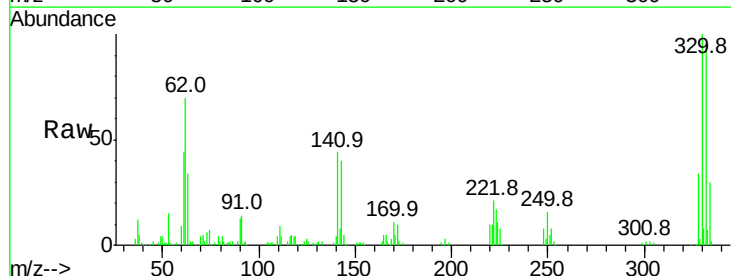


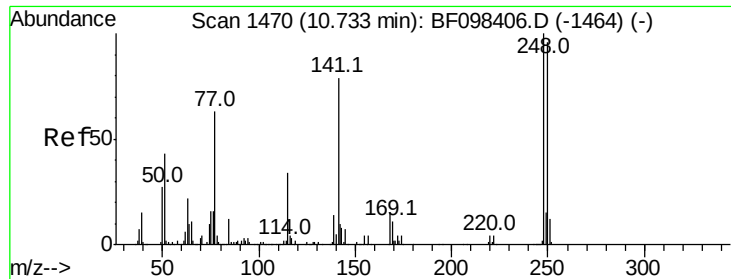




#66
4-Bromophenyl-phenylether
Concen: 2.470 ng
RT: 10.46 min Scan# 1423
Delta R.T. -0.24 min
Lab File: BF098627.D
Acq: 19 Sep 2017 3:37

Instrument :
BNA_F
ClientSampleId :

Tot Ion:248 Resp: 8369
Ion Ratio Lower Upper
248 100
250 203.4 76.8 115.2#
141 578.0 68.6 103.0#

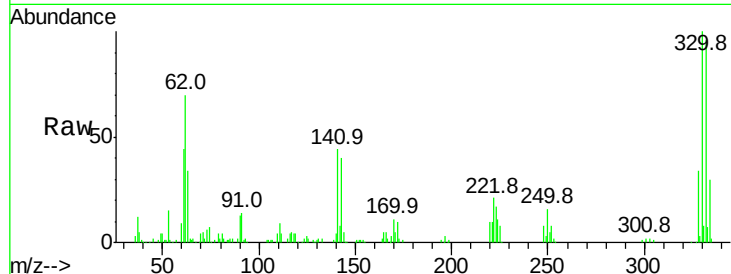


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

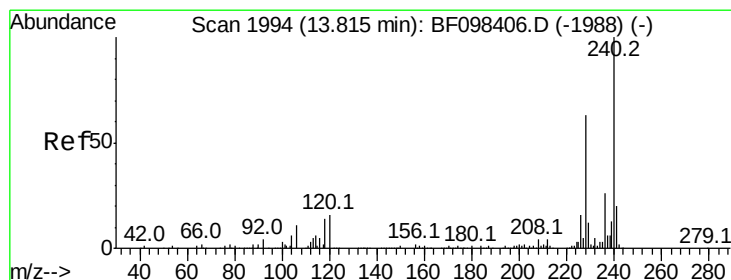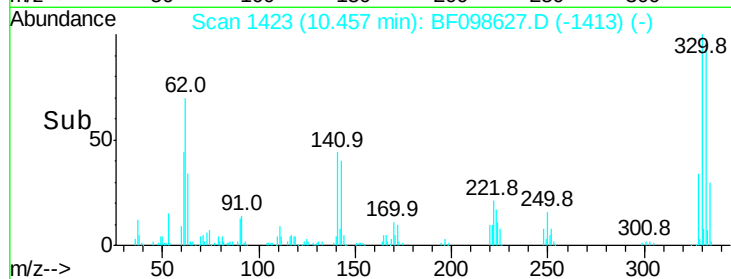
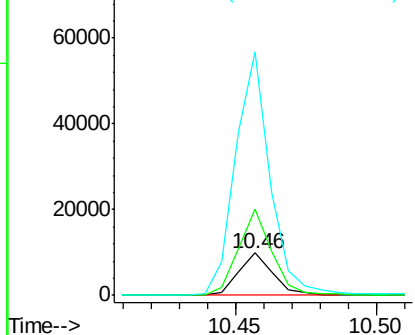



#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.78 min Scan# 1988
Delta R.T. -0.01 min
Lab File: BF098627.D
Acq: 19 Sep 2017 3:37

Tgt Ion:240 Resp: 236891
Ion Ratio Lower Upper
240 100
120 13.0 5.8 8.8#
236 26.8 20.5 30.7

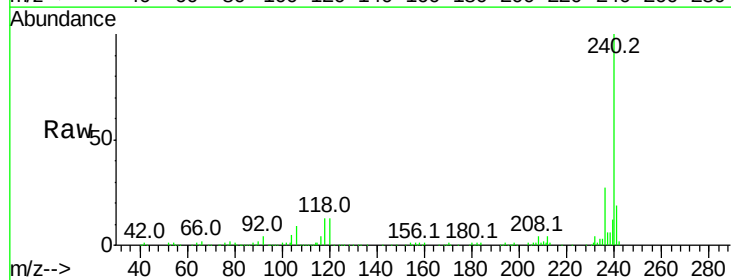

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



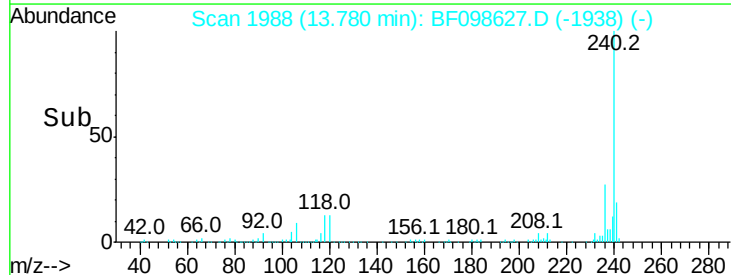
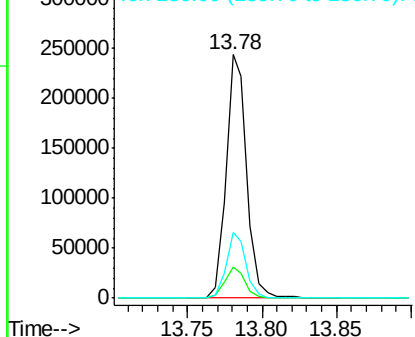




#78
 Terphenyl-d14
 Concen: 80.815 ng
 RT: 12.73 min Scan# 1810
 Delta R.T. 0.00 min
 Lab File: BF098627.D
 Acq: 19 Sep 2017 3:37

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:244 Resp: 886942
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.0 9.0
 122 12.9 10.3 15.5

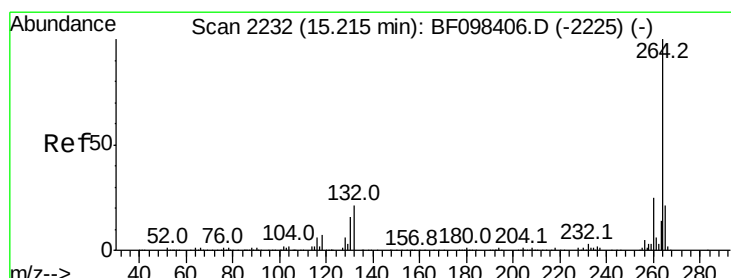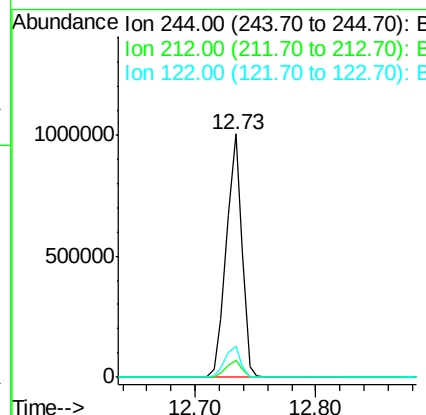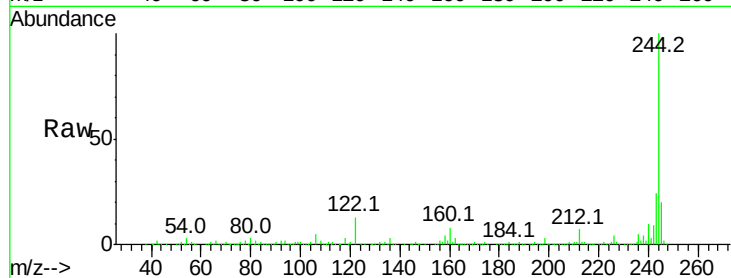

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.18 min Scan# 2226
 Delta R.T. 0.01 min
 Lab File: BF098627.D
 Acq: 19 Sep 2017 3:37

Tgt Ion:264 Resp: 231443
 Ion Ratio Lower Upper
 264 100
 260 25.7 19.5 29.3
 265 22.4 17.2 25.8

