
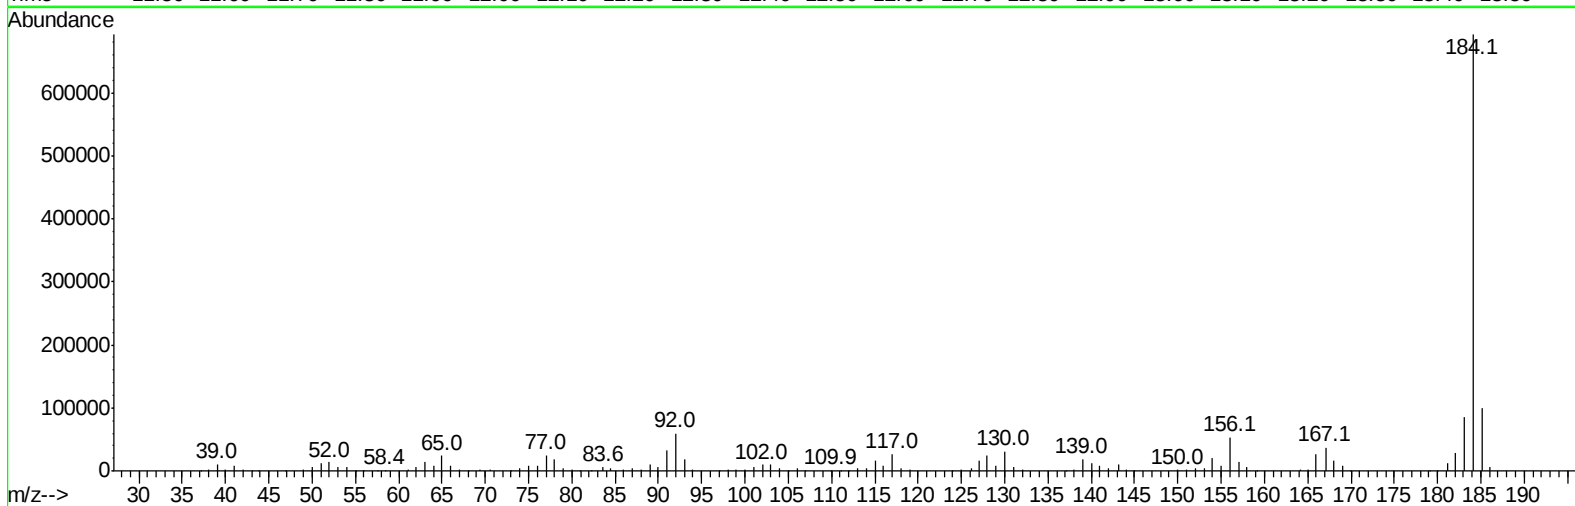


Data Path : Z:\HPCHEM1\BNA F\DATA\BF091817\
 Data File : BF098595.D
 Acq On : 18 Sep 2017 11:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 09:13:46 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 18 13:37:24 2017
 Response via : Initial Calibration

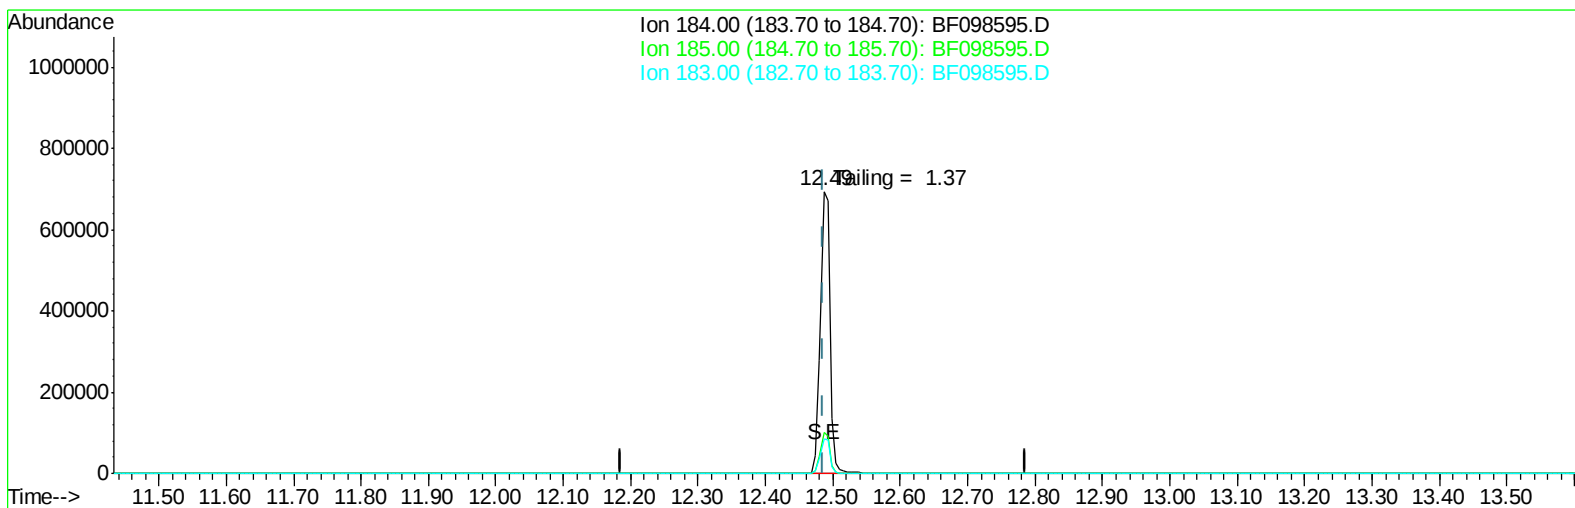

TIC: BF098595.D

(76) Benzidine



12.486min (-0.000) 0.00ng

response 665965

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.47#
183.00	12.20	12.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF091817\
Data File : BF098595.D
Acq On : 18 Sep 2017 11:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 09:13:46 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 18 13:37:24 2017
Response via : Initial Calibration

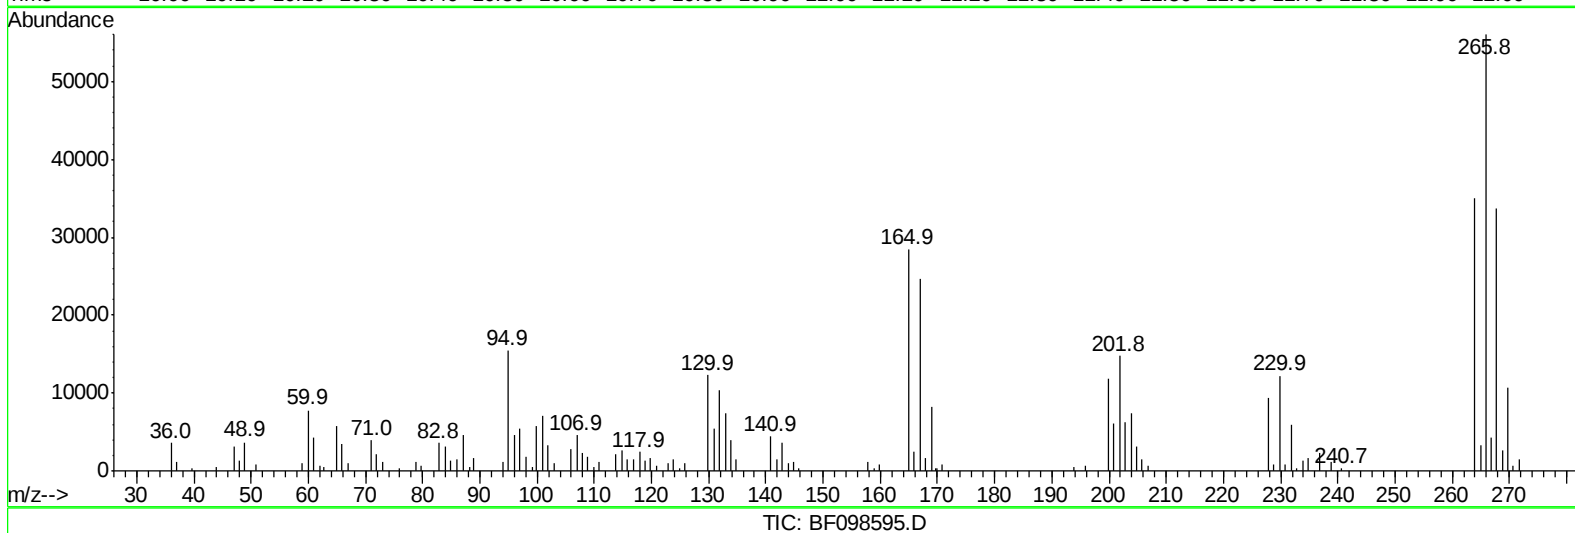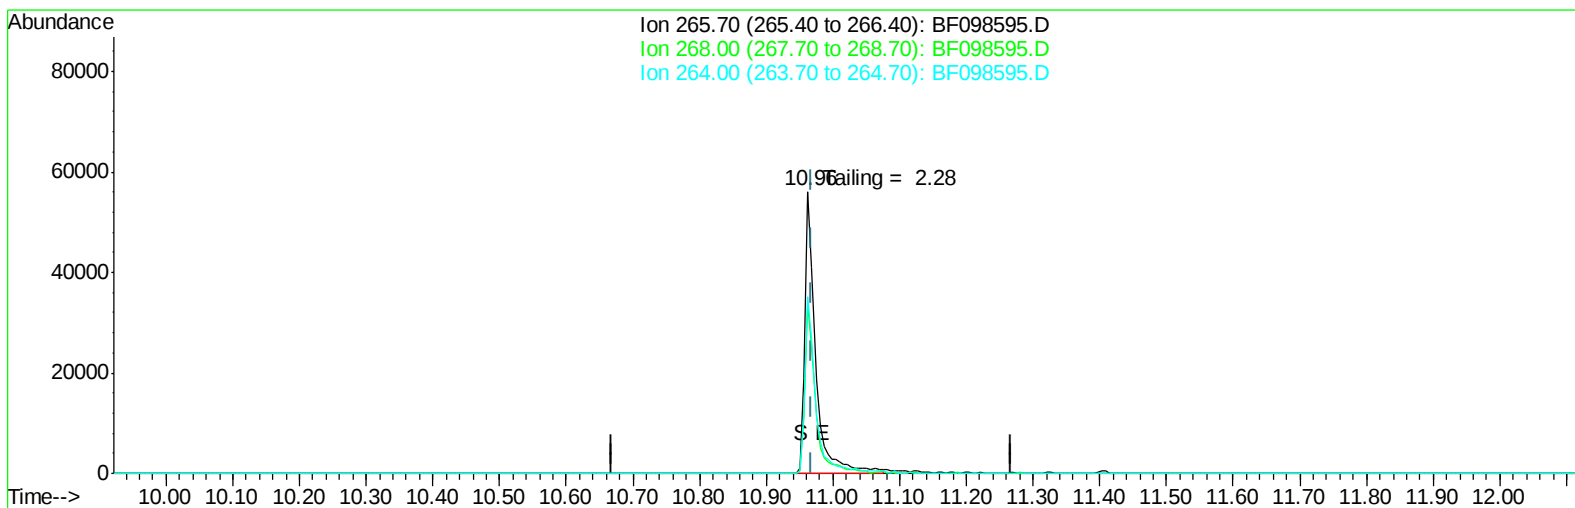

(69) Pentachlorophenol (C)

10.963min (-0.006) 23249.36ng

response 62795

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.11
264.00	64.60	62.59
0.00	0.00	0.00