
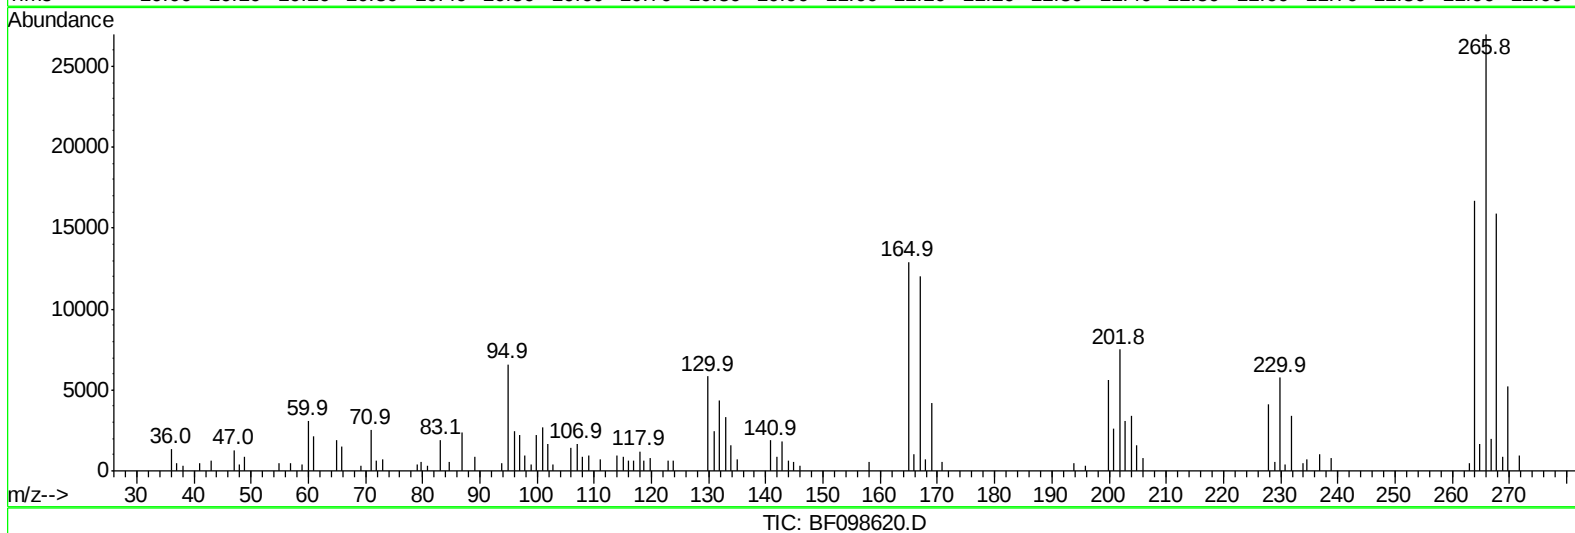


Data Path : Z:\HPCHEM1\BNA F\DATA\BF091817\
Data File : BF098620.D
Acq On : 19 Sep 2017 00:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 09:15:17 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 18 13:37:24 2017
Response via : Initial Calibration

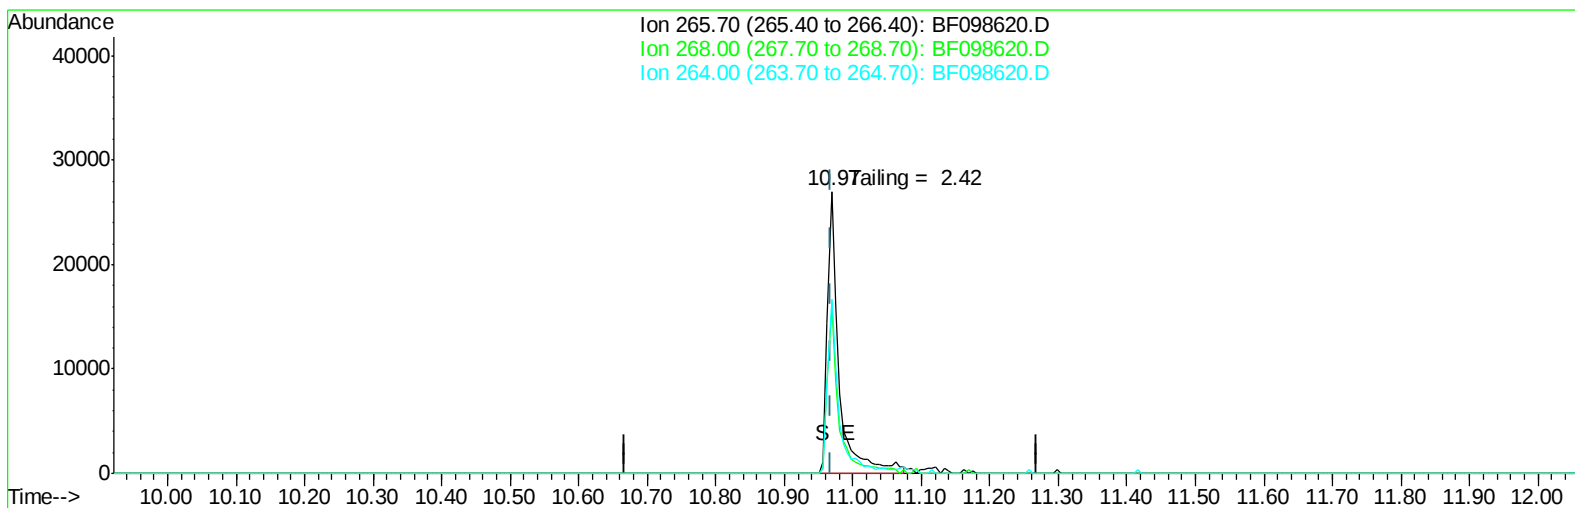

(69) Pentachlorophenol (C)



10.969min (-0.000) 21120.62ng

response 30443

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	58.96
264.00	64.60	61.79
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF091817\
Data File : BF098620.D
Acq On : 19 Sep 2017 00:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 09:15:17 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 18 13:37:24 2017
Response via : Initial Calibration

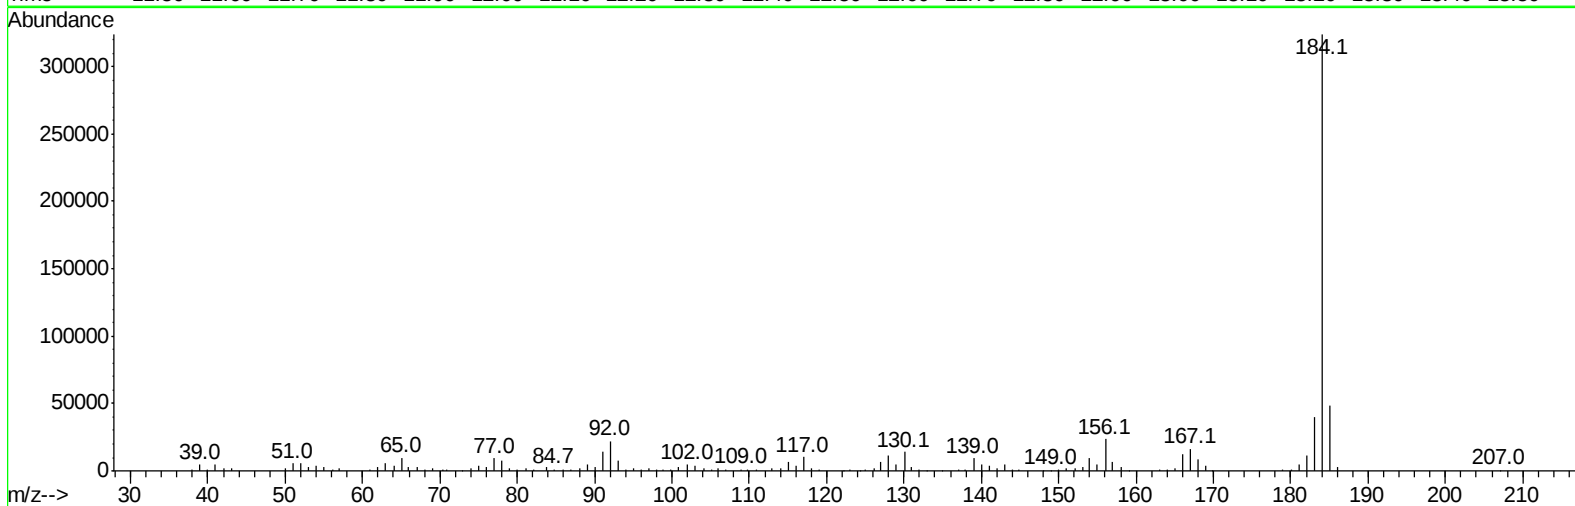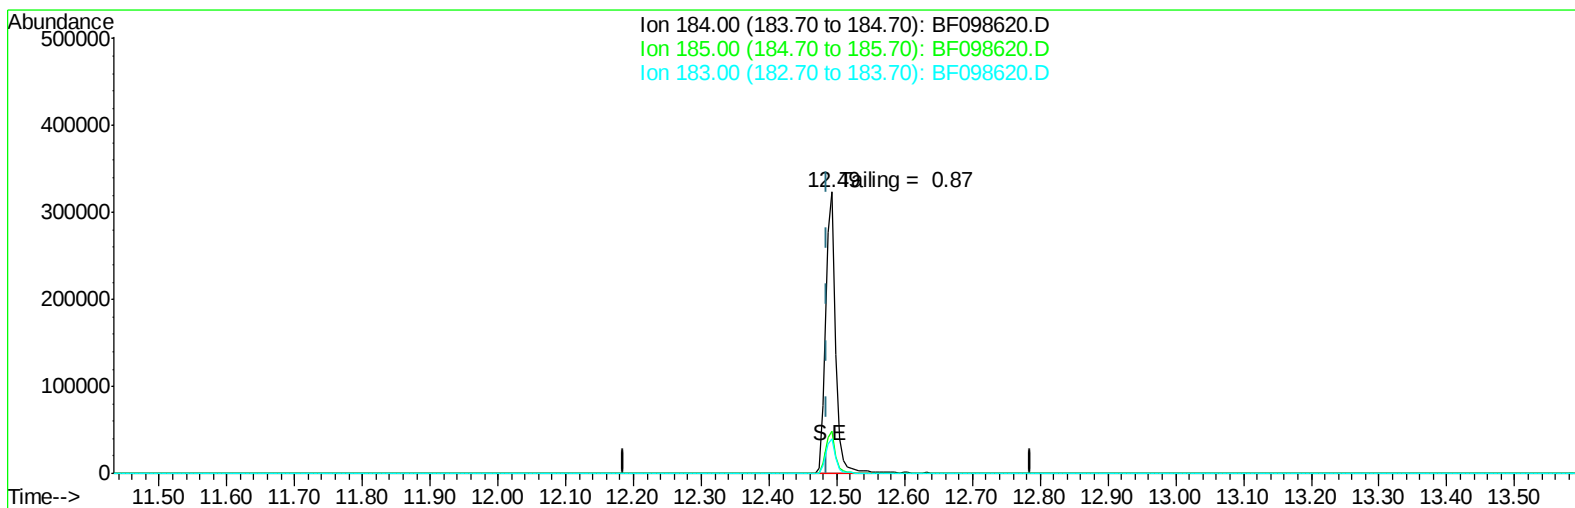

TIC: BF098620.D

(76) Benzidine

12.492min (+0.006) 0.00ng

response 322601

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.11#
183.00	12.20	12.34
0.00	0.00	0.00