

Data Path : Z:\HPCHEM1\BNA F\DATA\BF091817\
 Data File : BF098626.D
 Acq On : 19 Sep 2017 3:09
 Operator : SJ/JU
 Sample : I5262-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 091417-SIDI-E-D-B

Quant Time: Sep 19 07:24:51 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 18 13:37:24 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.63	152	100697	20.00	ng	0.00
21) Naphthalene-d8	7.92	136	402972	20.00	ng	0.00
38) Acenaphthene-d10	9.67	164	182135	20.00	ng	0.00
63) Phenanthrene-d10	11.15	188	376018	20.00	ng	0.00
75) Chrysene-d12	13.79	240	250871	20.00	ng	0.00
86) Perylene-d12	15.18	264	240292	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.24	112	287613	42.23	ng	0.00
7) Phenol-d6	6.29	99	228414	26.41	ng	0.00
23) Nitrobenzene-d5	7.20	82	606448	83.90	ng	0.00
41) 2,4,6-Tribromophenol	10.46	330	115302	94.85	ng	0.00
44) 2-Fluorobiphenyl	9.00	172	1098026	102.18	ng	0.00
78) Terphenyl-d14	12.73	244	914162	78.65	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.39	163	48249	3.422	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF091817\
Data File : BF098626.D
Acq On : 19 Sep 2017 3:09
Operator : SJ/JU
Sample : I5262-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
091417-SIDI-E-D-B

Quant Time: Sep 19 07:24:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 18 13:37:24 2017
Response via : Initial Calibration

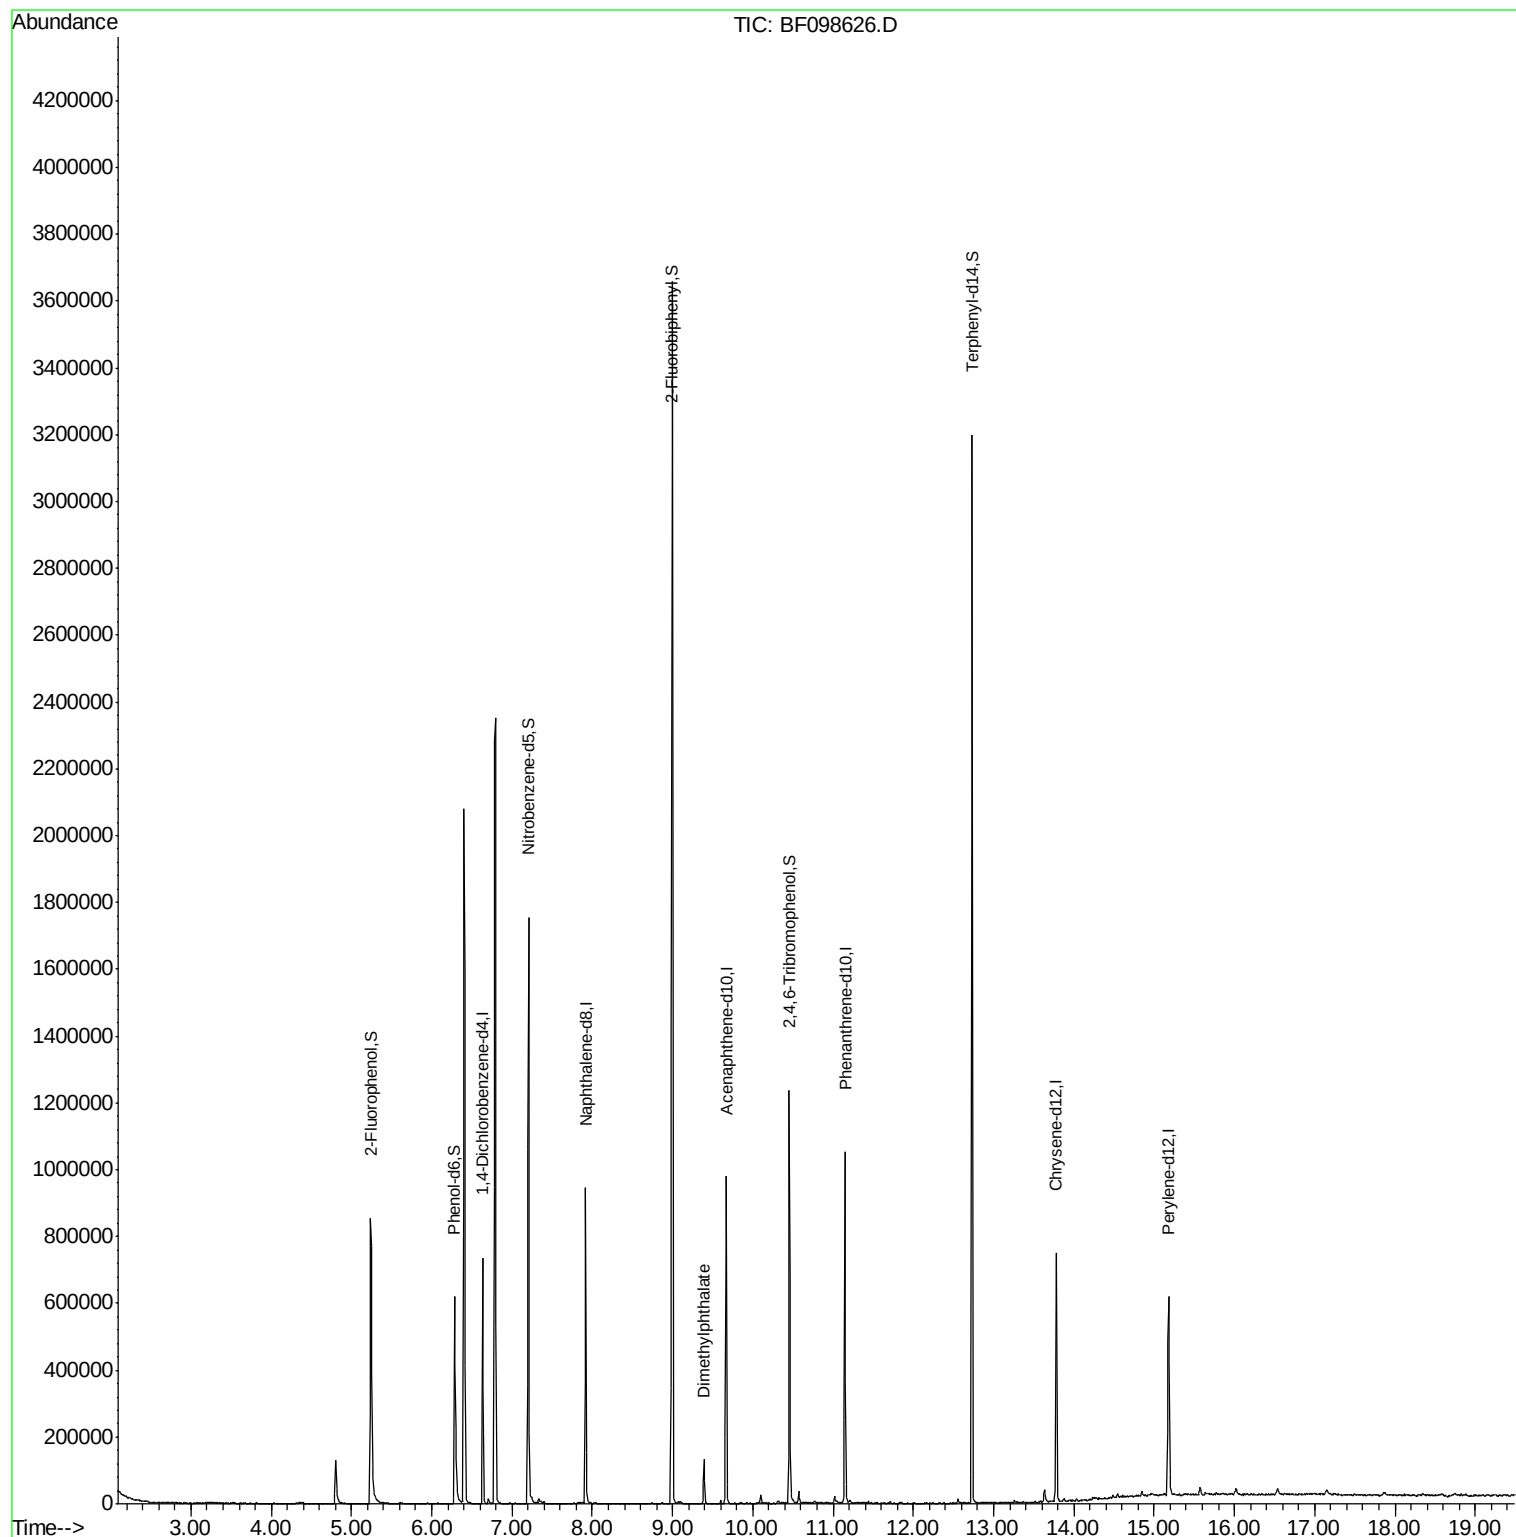

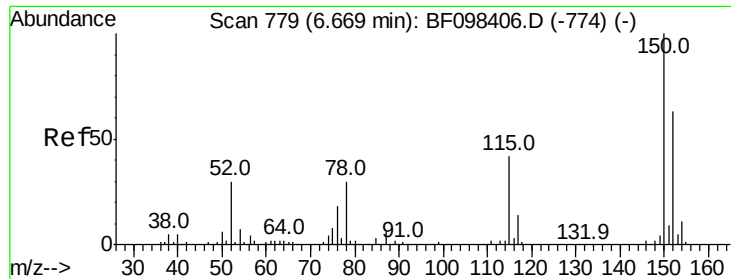

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 6.63 min Scan# 773

Delta R.T. -0.00 min

Lab File: BF098626.D

Acq: 19 Sep 2017 3:09

Instrument :

BNA_F

ClientSampleId :

091417-SIDI-E-D-B


Tot Ion:152 Resp: 100697

Ion Ratio Lower Upper

152 100

150 156.7 126.2 189.2




115 65.7 52.2 78.2

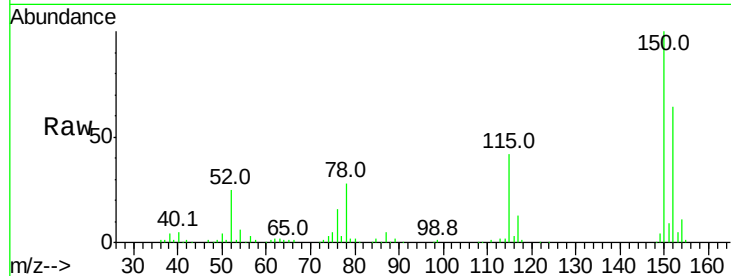

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

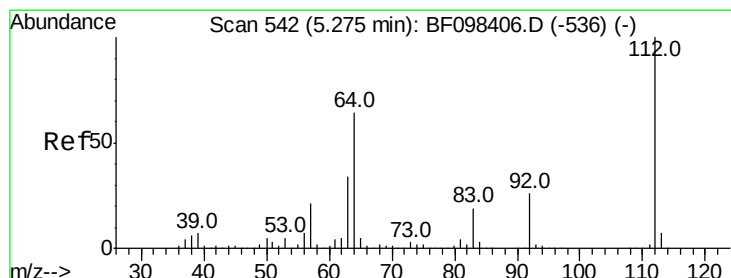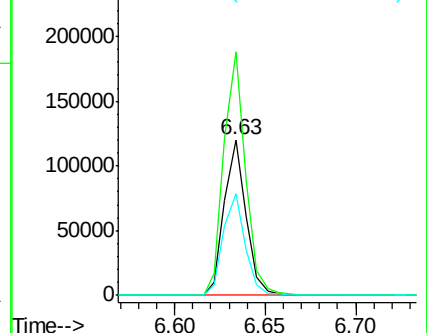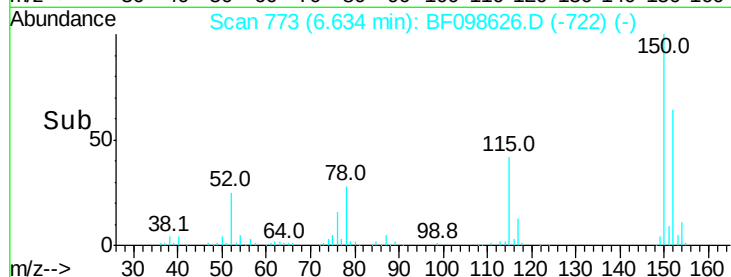

#5

2-Fluorophenol

Concen: 42.230 ng

RT: 5.24 min Scan# 536

Delta R.T. -0.00 min

Lab File: BF098626.D

Acq: 19 Sep 2017 3:09


Tgt Ion:112 Resp: 287613

Ion Ratio Lower Upper

112 100

64 65.3 46.0 69.0



63 34.5 23.4 35.0

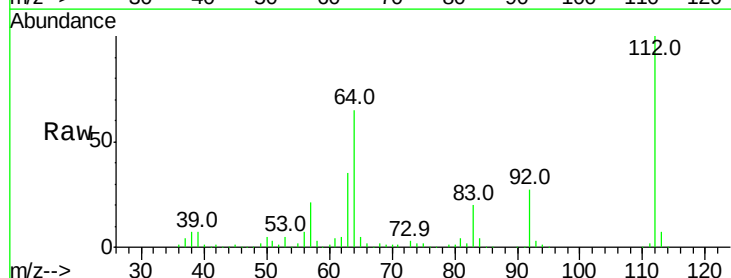


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

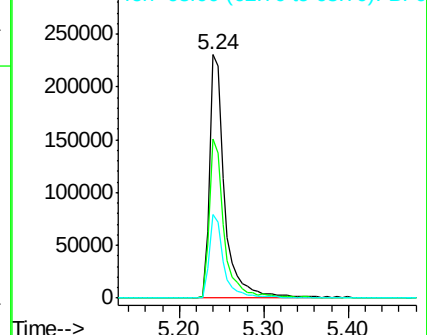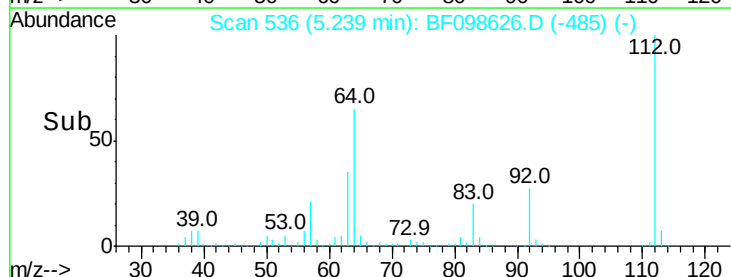

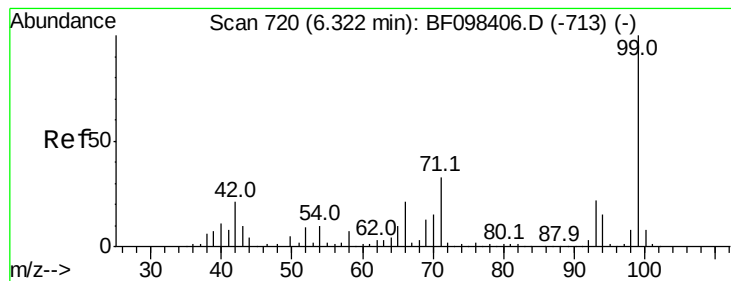

#7

Phenol-d6

Concen: 26.415 ng

RT: 6.29 min Scan# 714

Delta R.T. -0.01 min

Lab File: BF098626.D

Acq: 19 Sep 2017 3:09

Instrument :

BNA_F

ClientSampleId :

091417-SIDI-E-D-B


Tot Ion: 99 Resp: 228414

Ion Ratio Lower Upper

99 100

42 19.7 13.5 20.3




71 34.5 24.5 36.7

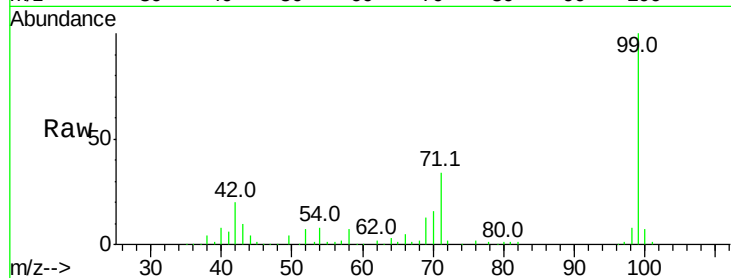

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

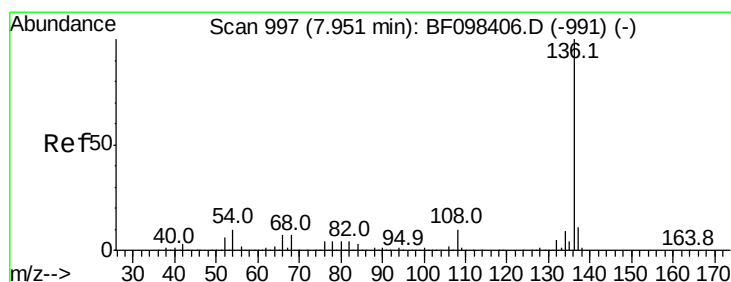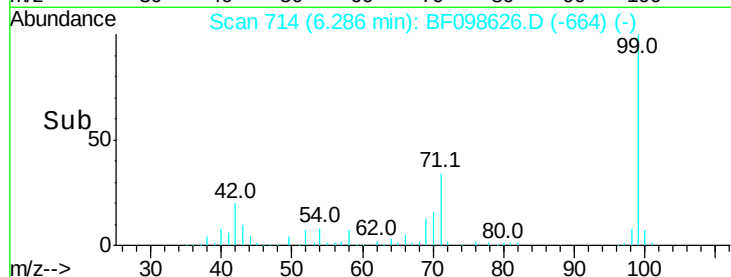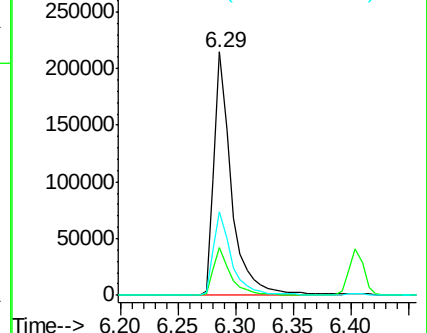

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.92 min Scan# 991

Delta R.T. -0.01 min

Lab File: BF098626.D

Acq: 19 Sep 2017 3:09

Tgt Ion: 136 Resp: 402972


Ion Ratio Lower Upper

136 100

137 11.3 8.5 12.7

54 9.8 4.9 7.3#

68 5.5 4.1 6.1


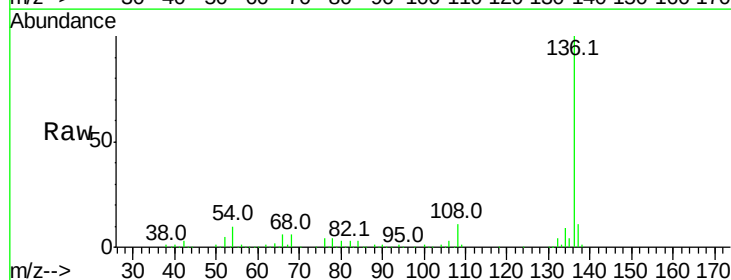



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

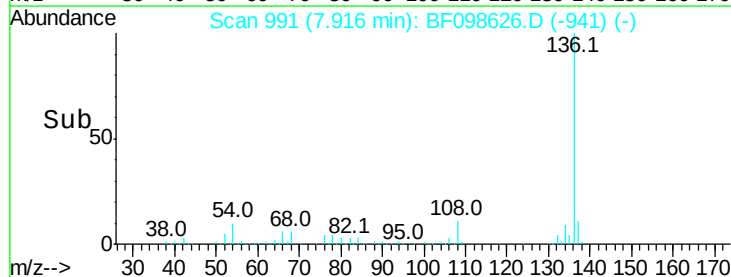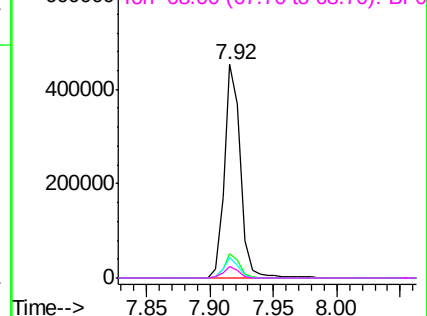

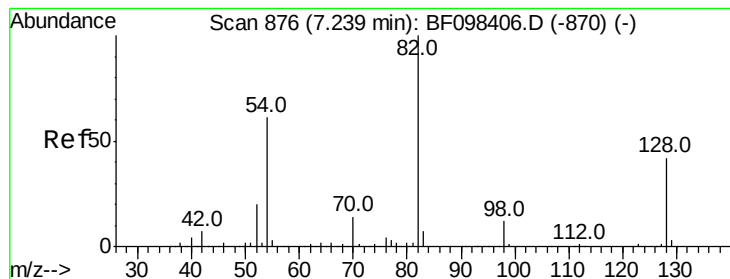

#23

Nitrobenzene-d5

Concen: 83.900 ng

RT: 7.20 min Scan# 870

Delta R.T. -0.01 min

Lab File: BF098626.D

Acq: 19 Sep 2017 3:09

Instrument :

BNA_F

ClientSampleId :

091417-SIDI-E-D-B


Tot Ion: 82 Resp: 606448

Ion Ratio Lower Upper




82 100

128 44.0 34.0 51.0

54 58.4 42.2 63.2

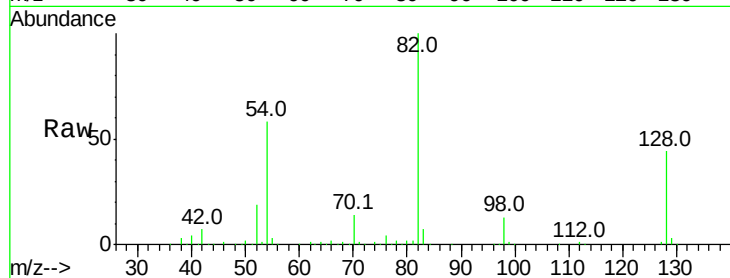

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

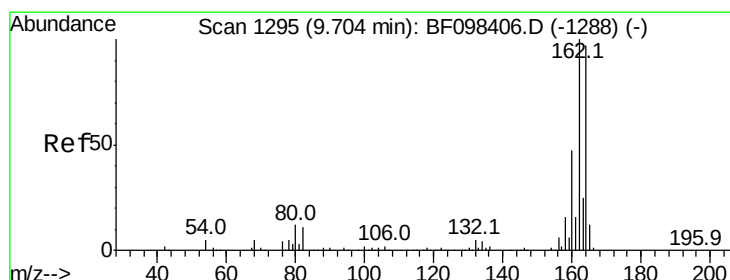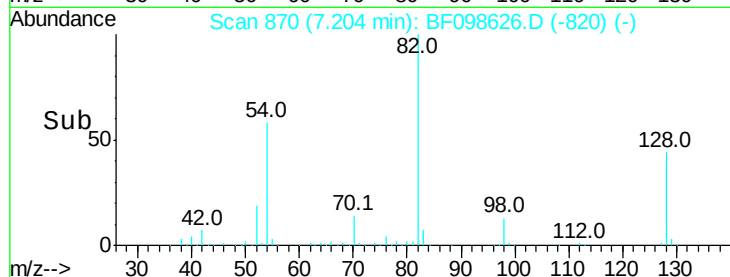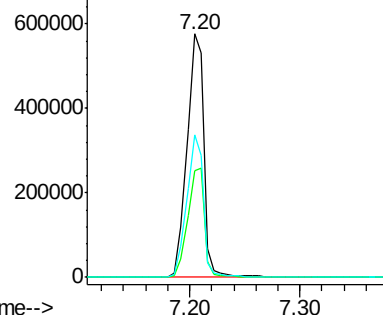

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.67 min Scan# 1289

Delta R.T. -0.00 min

Lab File: BF098626.D

Acq: 19 Sep 2017 3:09


Tgt Ion: 164 Resp: 182135

Ion Ratio Lower Upper



164 100


162 105.8 82.6 123.8

160 48.0 36.2 54.2

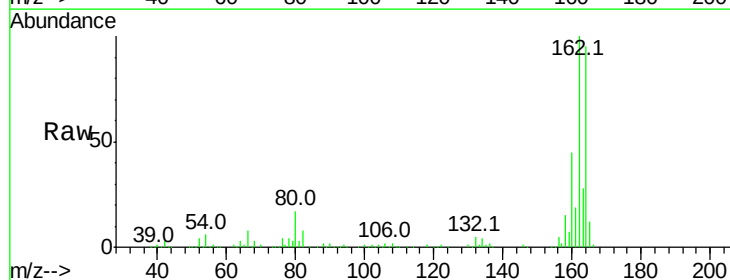

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

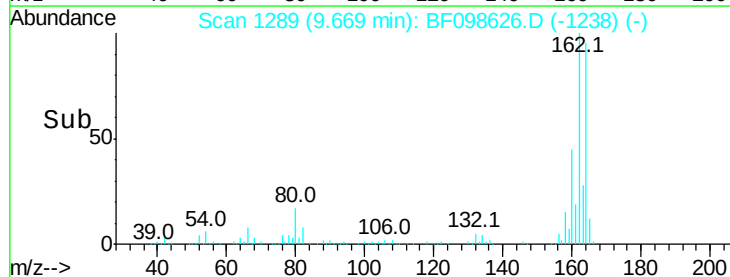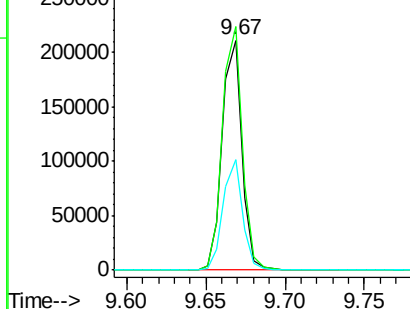


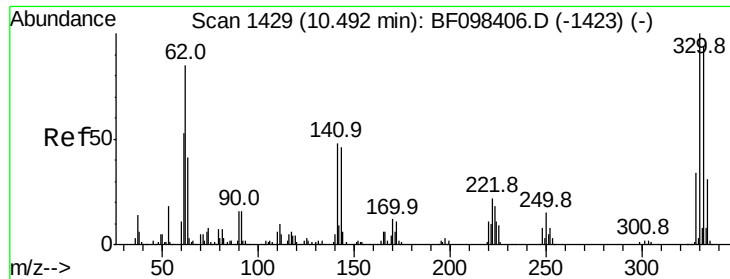




#41
 2,4,6-Tribromophenol
 Concen: 94.852 ng
 RT: 10.46 min Scan# 1423
 Delta R.T. -0.01 min
 Lab File: BF098626.D
 Acq: 19 Sep 2017 3:09

Instrument :
 BNA_F
 ClientSampleId :
 091417-SIDI-E-D-B

Tot Ion:330 Resp: 115302
 Ion Ratio Lower Upper
 330 100
 332 98.0 76.6 115.0
 141 43.5 31.4 47.2

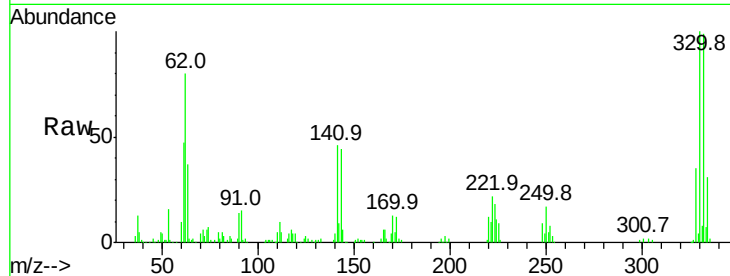


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

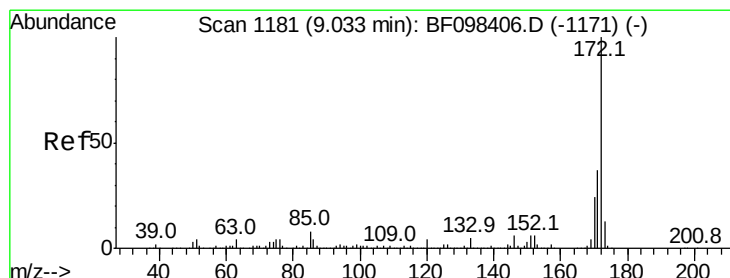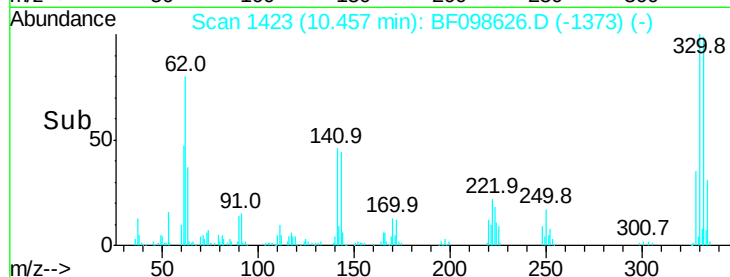
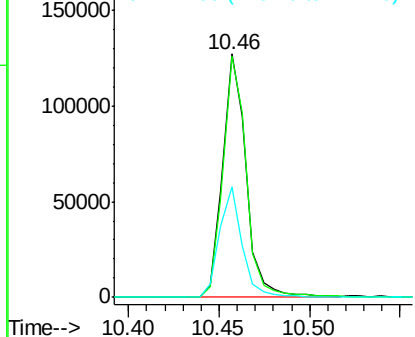



#44
 2-Fluorobiphenyl
 Concen: 102.180 ng
 RT: 9.00 min Scan# 1175
 Delta R.T. -0.00 min
 Lab File: BF098626.D
 Acq: 19 Sep 2017 3:09

Tgt Ion:172 Resp: 1098026
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.6 44.4
 170 24.1 19.8 29.8

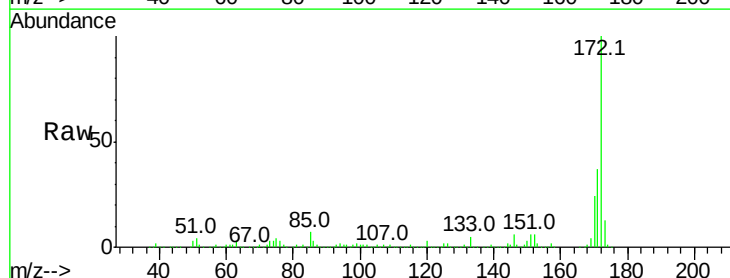

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



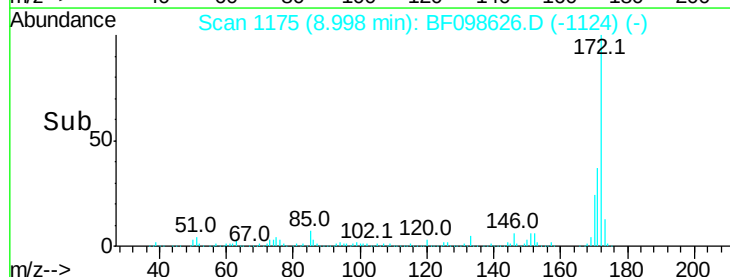
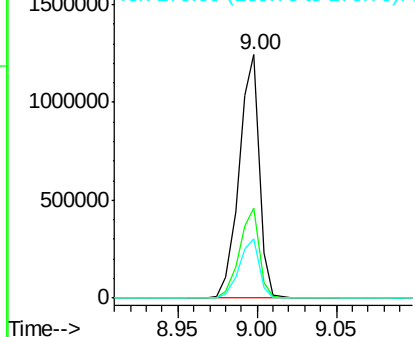


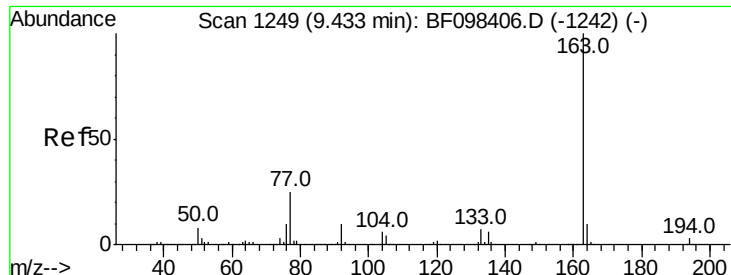

#49
Dimethylphthalate
Concen: 3.422 ng
RT: 9.39 min Scan# 1242
Delta R.T. -0.01 min
Lab File: BF098626.D
Acq: 19 Sep 2017 3:09




Instrument :
BNA_F
ClientSampleId :
091417-SIDI-E-D-B


Tot Ion:163 Resp: 48249
Ion Ratio Lower Upper
163 100
194 3.3 2.6 4.0
164 10.7 8.4 12.6

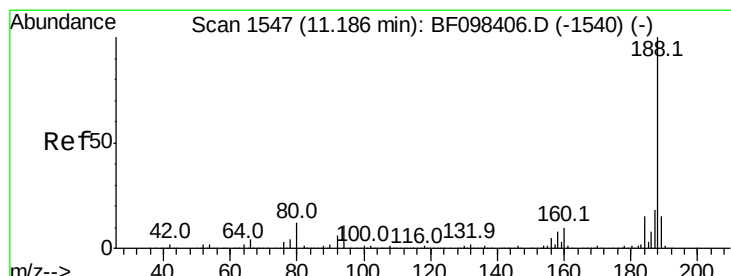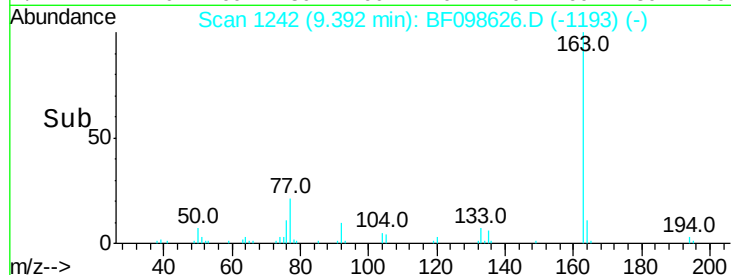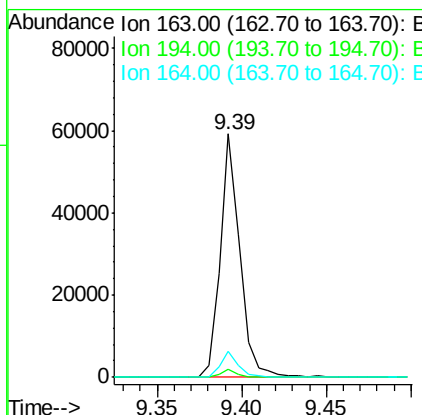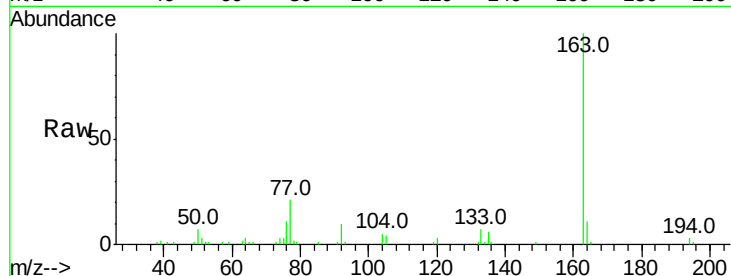

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.15 min Scan# 1541
Delta R.T. -0.00 min
Lab File: BF098626.D
Acq: 19 Sep 2017 3:09

Tgt Ion:188 Resp: 376018
Ion Ratio Lower Upper
188 100
94 8.8 9.4 14.2#
80 9.5 10.2 15.2#

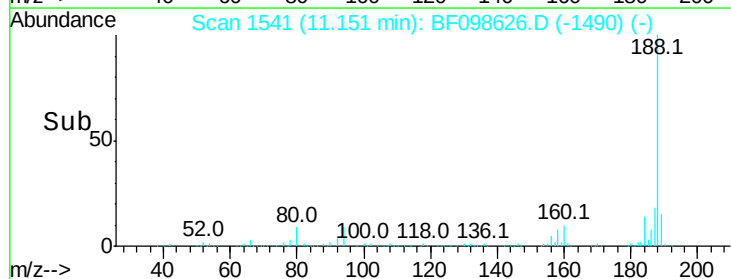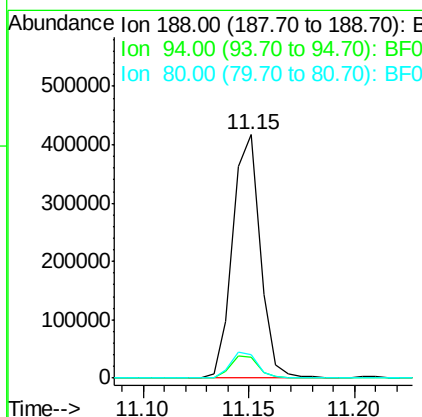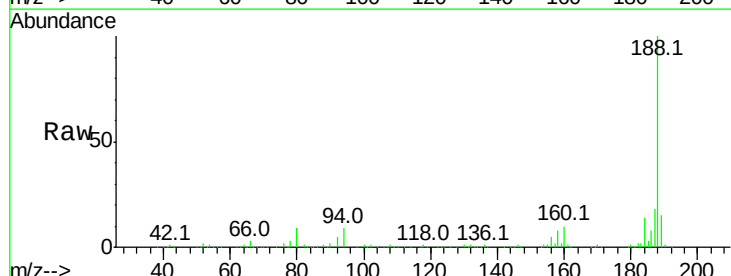

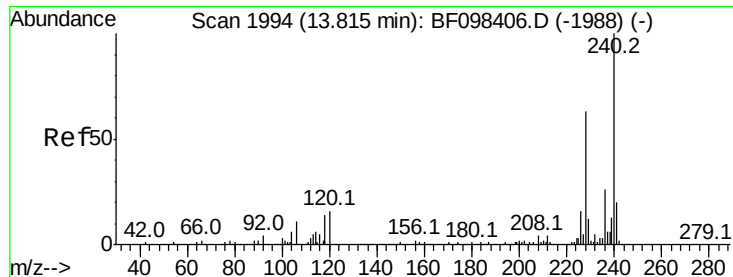

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.79 min Scan# 1989

Delta R.T. -0.00 min

Lab File: BF098626.D

Acq: 19 Sep 2017 3:09

Instrument :

BNA_F

ClientSampleId :

091417-SIDI-E-D-B


Tot Ion:240 Resp: 250871

Ion Ratio Lower Upper

240 100

120 11.7 5.8 8.8#




236 25.6 20.5 30.7

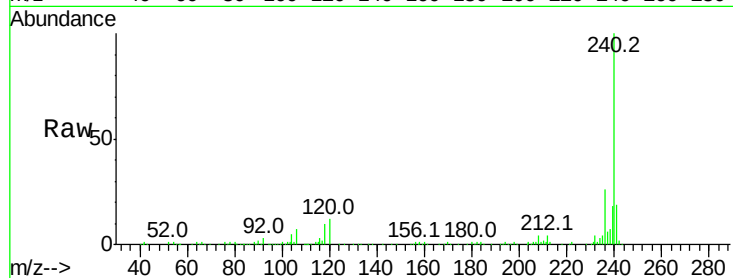

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

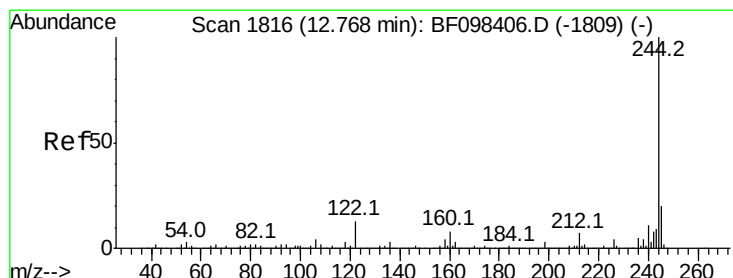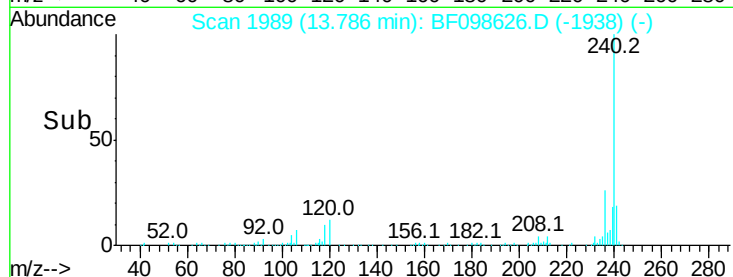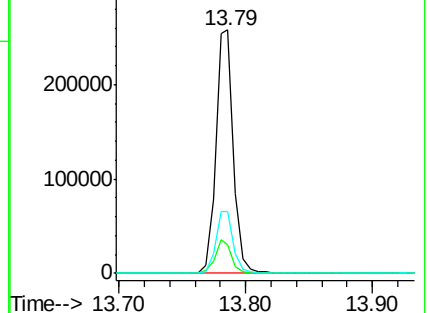

#78

Terphenyl-d14

Concen: 78.653 ng

RT: 12.73 min Scan# 1810

Delta R.T. -0.00 min

Lab File: BF098626.D

Acq: 19 Sep 2017 3:09


Tgt Ion:244 Resp: 914162

Ion Ratio Lower Upper

244 100

212 7.5 6.0 9.0



122 12.9 10.3 15.5

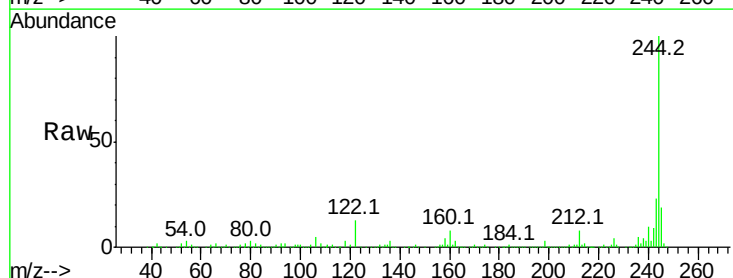


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

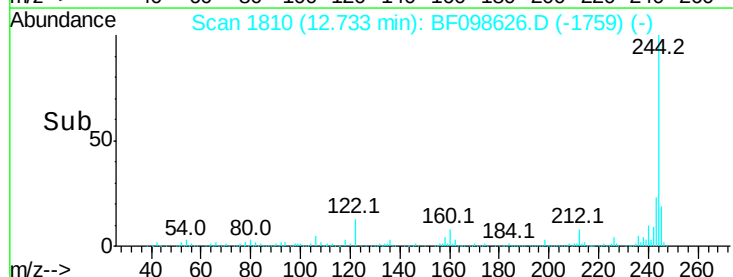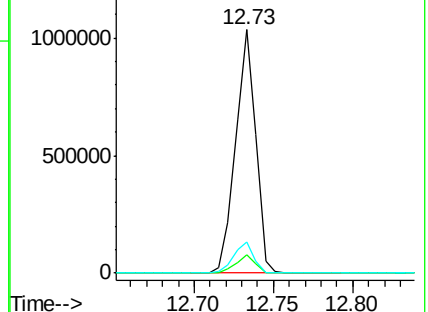


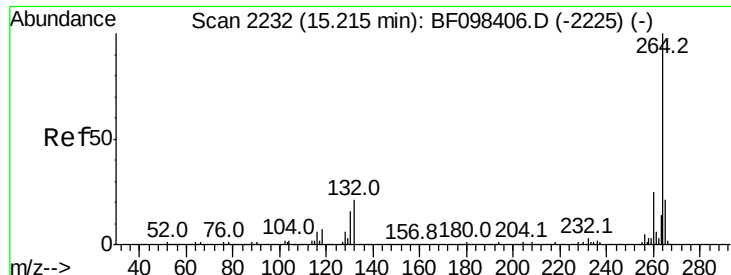

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.18 min Scan# 2226
 Delta R.T. 0.01 min
 Lab File: BF098626.D
 Acq: 19 Sep 2017 3:09

Instrument :
 BNA_F
 ClientSampleId :
 091417-SIDI-E-D-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.5	29.3
265	21.1	17.2	25.8

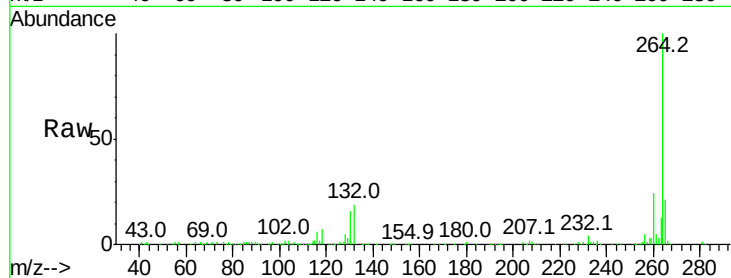

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

