


Data Path : Z:\HPCHEM1\BNA F\Data\BF091817\
 Data File : BF098595.D
 Acq On : 18 Sep 2017 11:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 18 13:37:24 2017

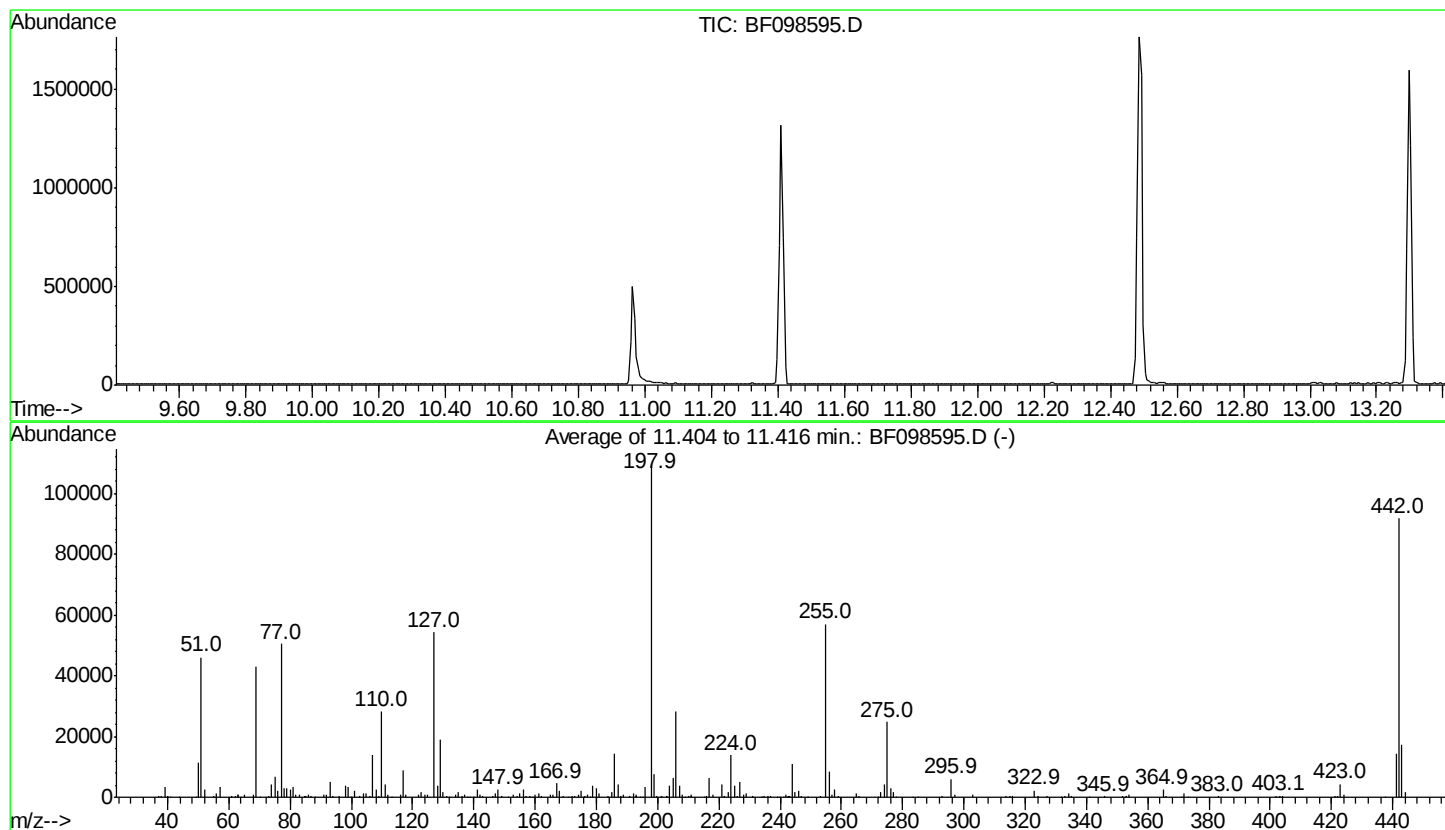

AutoFind: Scans 1584, 1585, 1586; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	46125	PASS
68	69	0.00	2	1.7	711	PASS
69	198	0.00	100	39.5	43064	PASS
70	69	0.00	2	0.3	117	PASS
127	198	10	80	49.7	54237	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109141	PASS
199	198	5	9	6.9	7567	PASS
275	198	10	60	22.7	24735	PASS
365	198	1	100	2.3	2505	PASS
441	442	0.01	24	15.6	14323	PASS
442	198	50	100	84.0	91690	PASS
443	442	15	24	18.8	17192	PASS