


Data Path : Z:\HPCHEM1\BNA F\Data\BF091817\
 Data File : BF098620.D
 Acq On : 19 Sep 2017 00:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 18 13:37:24 2017

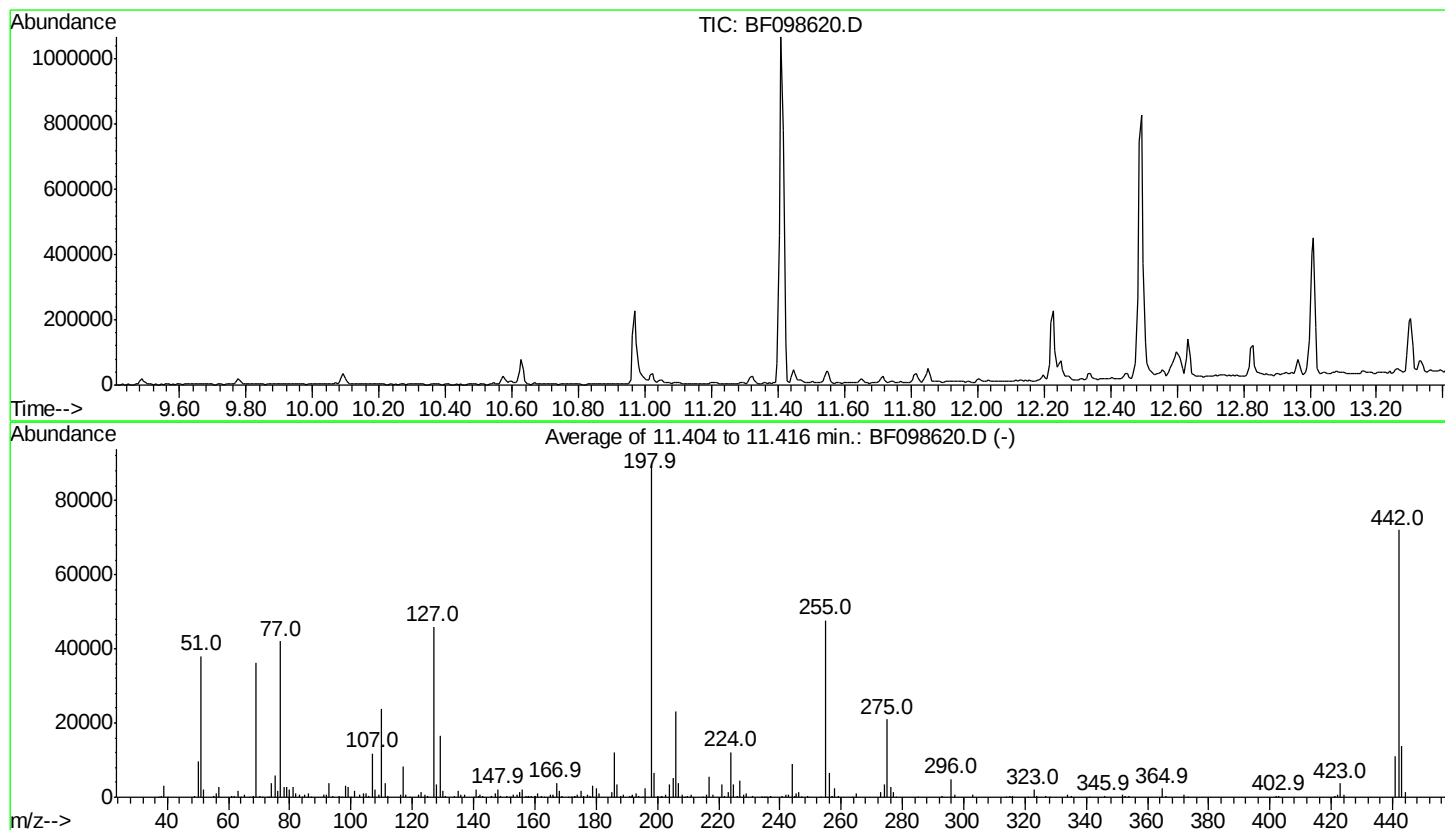

AutoFind: Scans 1584, 1585, 1586; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	38040	PASS
68	69	0.00	2	1.3	479	PASS
69	198	0.00	100	40.7	36356	PASS
70	69	0.00	2	0.8	288	PASS
127	198	10	80	51.4	45957	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89376	PASS
199	198	5	9	7.4	6585	PASS
275	198	10	60	23.5	21047	PASS
365	198	1	100	2.6	2366	PASS
441	442	0.01	24	15.5	11183	PASS
442	198	50	100	80.5	71960	PASS
443	442	15	24	19.2	13837	PASS