

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091820\
 Data File : BF121610.D
 Acq On : 18 Sep 2020 11:13
 Operator : JU/CG
 Sample : PB131684BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB131684BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.069	502	507	522	rVB	74280	101785	1.72%	0.295%
2	5.457	568	573	576	rBV	3816743	3777039	63.91%	10.953%
3	6.457	738	743	746	rBV	3396255	3825378	64.73%	11.093%
4	6.822	801	805	808	rBV	1209578	1018117	17.23%	2.952%
5	7.381	895	900	904	rBV	2271667	2772633	46.91%	8.041%
6	8.104	1017	1023	1039	rBV	1232295	1362944	23.06%	3.952%
7	9.180	1199	1206	1209	rBV	4279488	4921375	83.27%	14.272%
8	9.857	1315	1321	1343	rVB	1507483	1612353	27.28%	4.676%
9	10.645	1448	1455	1477	rBV	2752958	3253666	55.05%	9.435%
10	11.339	1567	1573	1580	rBV	1683207	1732060	29.31%	5.023%
11	12.745	1809	1812	1816	rVB	76927	67020	1.13%	0.194%
12	12.933	1836	1844	1847	rBV	5575292	5910092	100.00%	17.139%
13	13.386	1893	1921	1923	rBV3	37797	149412	2.53%	0.433%
14	13.451	1930	1932	1937	rVB2	78238	67218	1.14%	0.195%
15	13.980	2017	2022	2035	rBV	1742977	1768736	29.93%	5.129%
16	14.998	2182	2195	2196	rBV4	36173	115692	1.96%	0.336%
17	15.080	2207	2209	2219	rVB2	78925	115450	1.95%	0.335%
18	15.433	2261	2269	2285	rBV	1149458	1756353	29.72%	5.093%
19	15.886	2342	2346	2351	rVB	43519	60823	1.03%	0.176%
20	16.380	2425	2430	2437	rBV2	41397	95105	1.61%	0.276%


Sum of corrected areas: 34483251

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091820\
Data File : BF121610.D
Acq On : 18 Sep 2020 11:13
Operator : JU/CG
Sample : PB131684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131684BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

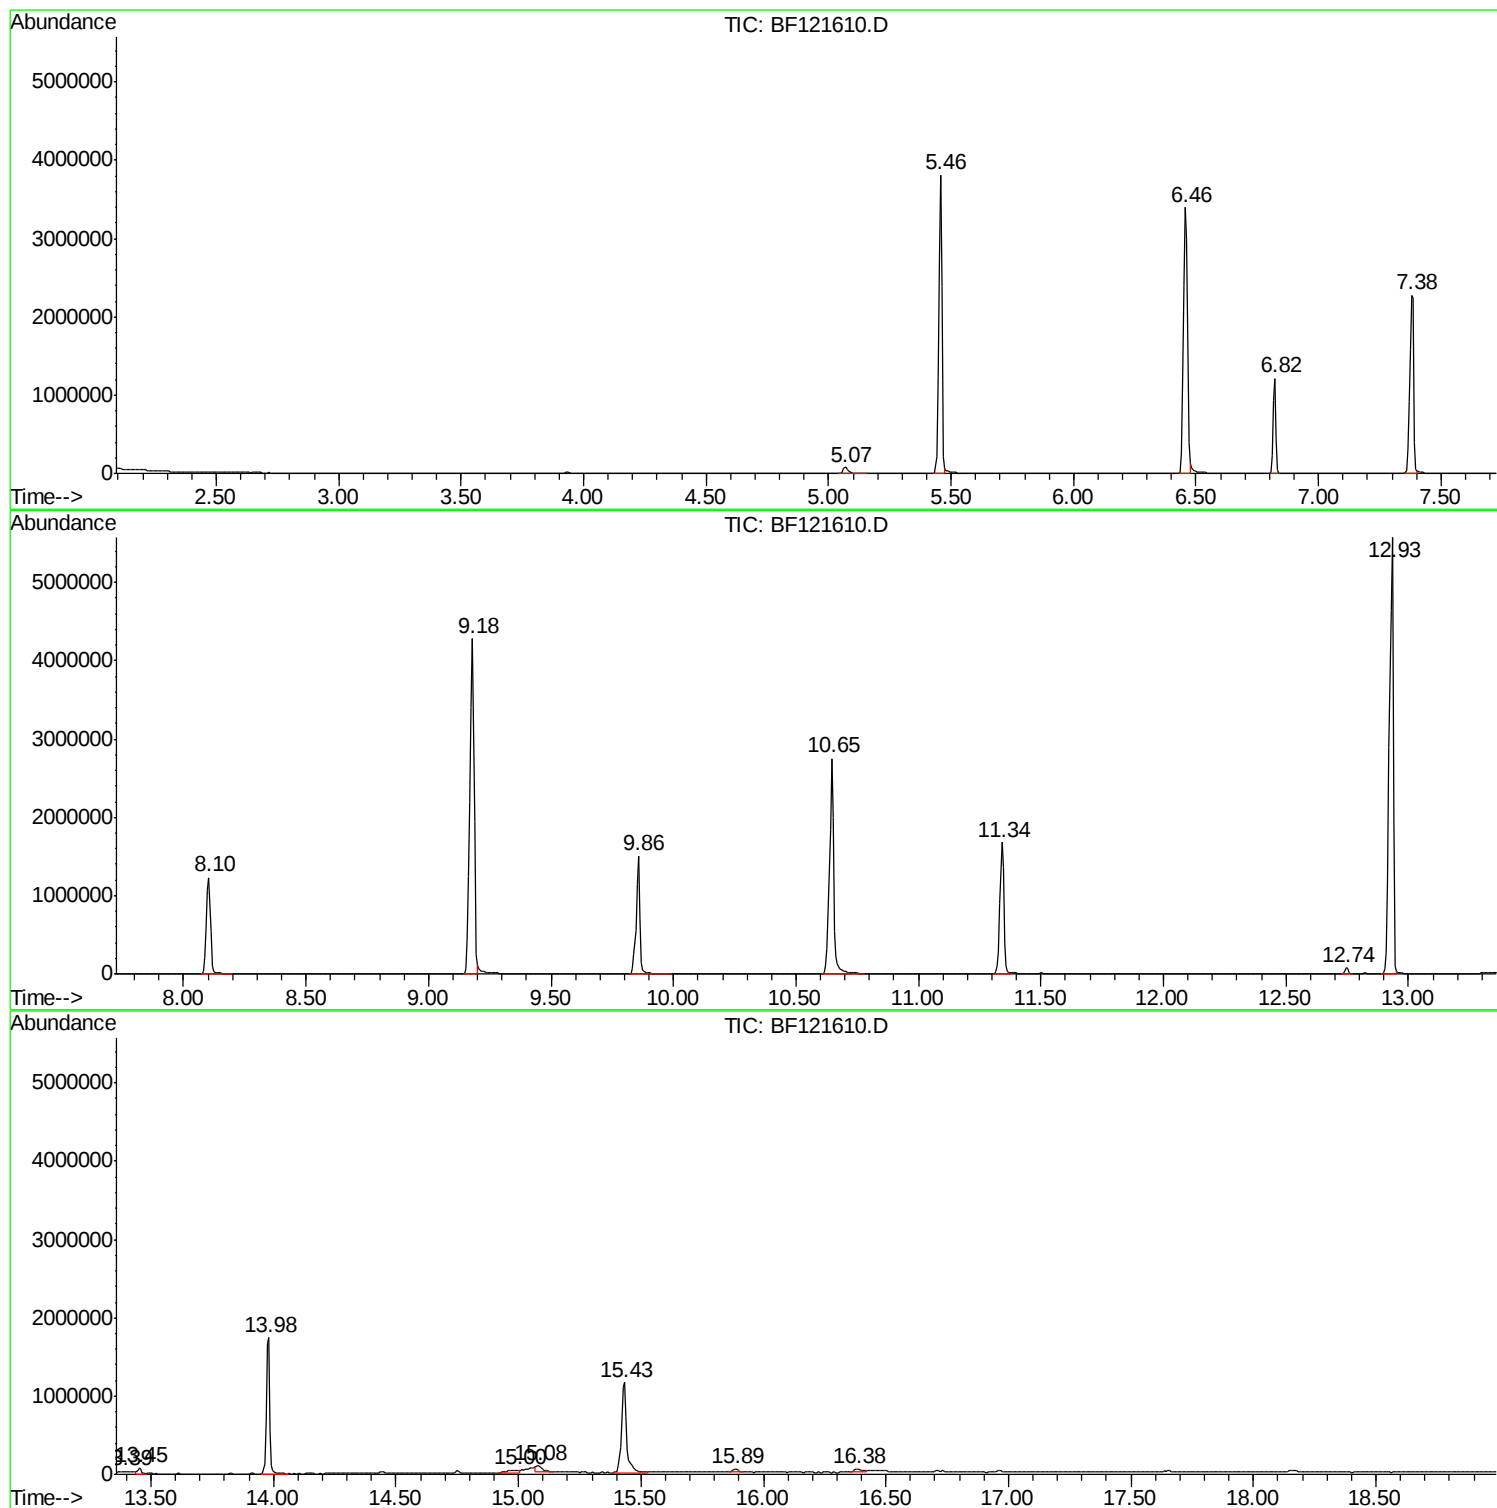

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091820\
Data File : BF121610.D
Acq On : 18 Sep 2020 11:13
Operator : JU/CG
Sample : PB131684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131684BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091820\
Data File : BF121610.D
Acq On : 18 Sep 2020 11:13
Operator : JU/CG
Sample : PB131684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131684BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc