

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091820\
 Data File : BF121615.D
 Acq On : 18 Sep 2020 16:17
 Operator : JU/CG
 Sample : L4059-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PAV-B33-091720-0-10

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.869	123	133	142	rVB	368298	587224	9.86%	1.430%
2	4.369	379	388	394	rBV3	40380	67787	1.14%	0.165%
3	4.446	396	401	407	rVB	86971	107151	1.80%	0.261%
4	4.634	426	433	440	rBV	150581	171974	2.89%	0.419%
5	5.063	500	506	518	rVB3	417761	738018	12.39%	1.797%
6	5.463	569	574	577	rBV	3808404	3949773	66.31%	9.620%
7	6.463	738	744	762	rBV	3295050	3742392	62.83%	9.115%
8	6.822	800	805	808	rBV	1098141	973460	16.34%	2.371%
9	7.387	894	901	904	rBV	2539369	3258773	54.71%	7.937%
10	7.492	914	919	929	rVB	82741	105002	1.76%	0.256%
11	8.104	1017	1023	1037	rBV	1162065	1328314	22.30%	3.235%
12	9.181	1199	1206	1209	rBV	4620156	5577471	93.64%	13.584%
13	9.857	1314	1321	1330	rBV	1455373	1498133	25.15%	3.649%
14	10.645	1447	1455	1469	rBV	2988742	3723820	62.52%	9.070%
15	11.339	1566	1573	1580	rBV	1489138	1561625	26.22%	3.803%
16	11.869	1656	1663	1672	rBV3	83647	163304	2.74%	0.398%
17	12.739	1809	1811	1819	rVB	64978	65217	1.09%	0.159%
18	12.933	1835	1844	1847	rBV	5387076	5956136	100.00%	14.507%
19	13.416	1917	1926	1927	rBV2	165364	361545	6.07%	0.881%
20	13.510	1927	1942	1943	rBV2	400282	1409935	23.67%	3.434%
21	13.610	1949	1959	1960	rBV	825189	2067621	34.71%	5.036%
22	13.980	2015	2022	2028	rBV	1351485	1632450	27.41%	3.976%
23	15.433	2264	2269	2277	rVB	904682	1192839	20.03%	2.905%
24	16.374	2427	2429	2439	rVB	69436	117495	1.97%	0.286%
25	16.974	2523	2531	2546	rVB3	171784	700891	11.77%	1.707%


Sum of corrected areas: 41058350

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091820\
Data File : BF121615.D
Acq On : 18 Sep 2020 16:17
Operator : JU/CG
Sample : L4059-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PAV-B33-091720-0-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

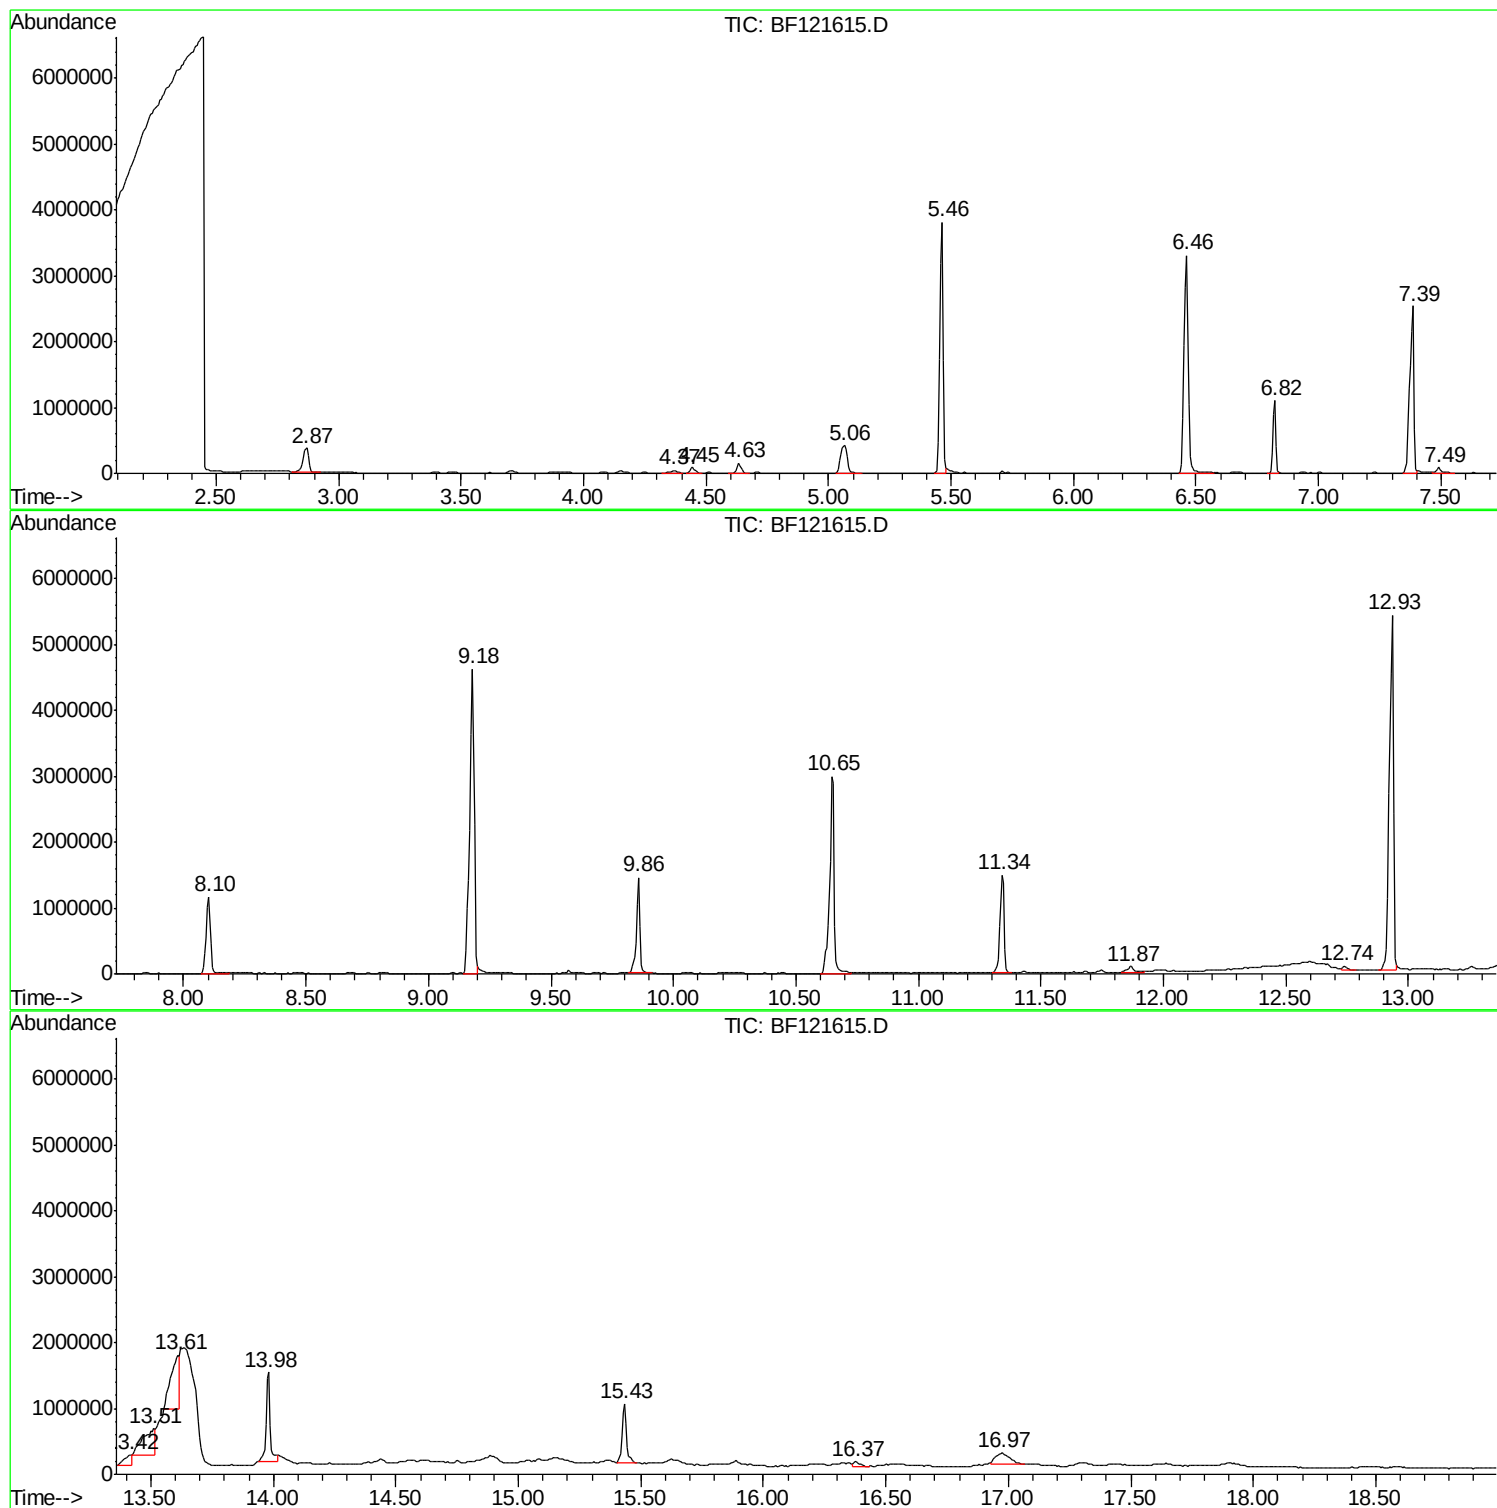

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091820\
Data File : BF121615.D
Acq On : 18 Sep 2020 16:17
Operator : JU/CG
Sample : L4059-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PAV-B33-091720-0-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091820\
Data File : BF121615.D
Acq On : 18 Sep 2020 16:17
Operator : JU/CG
Sample : L4059-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PAV-B33-091720-0-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc