


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091820\
 Data File : BF121608.D
 Acq On : 18 Sep 2020 10:02
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 10 16:47:54 2020

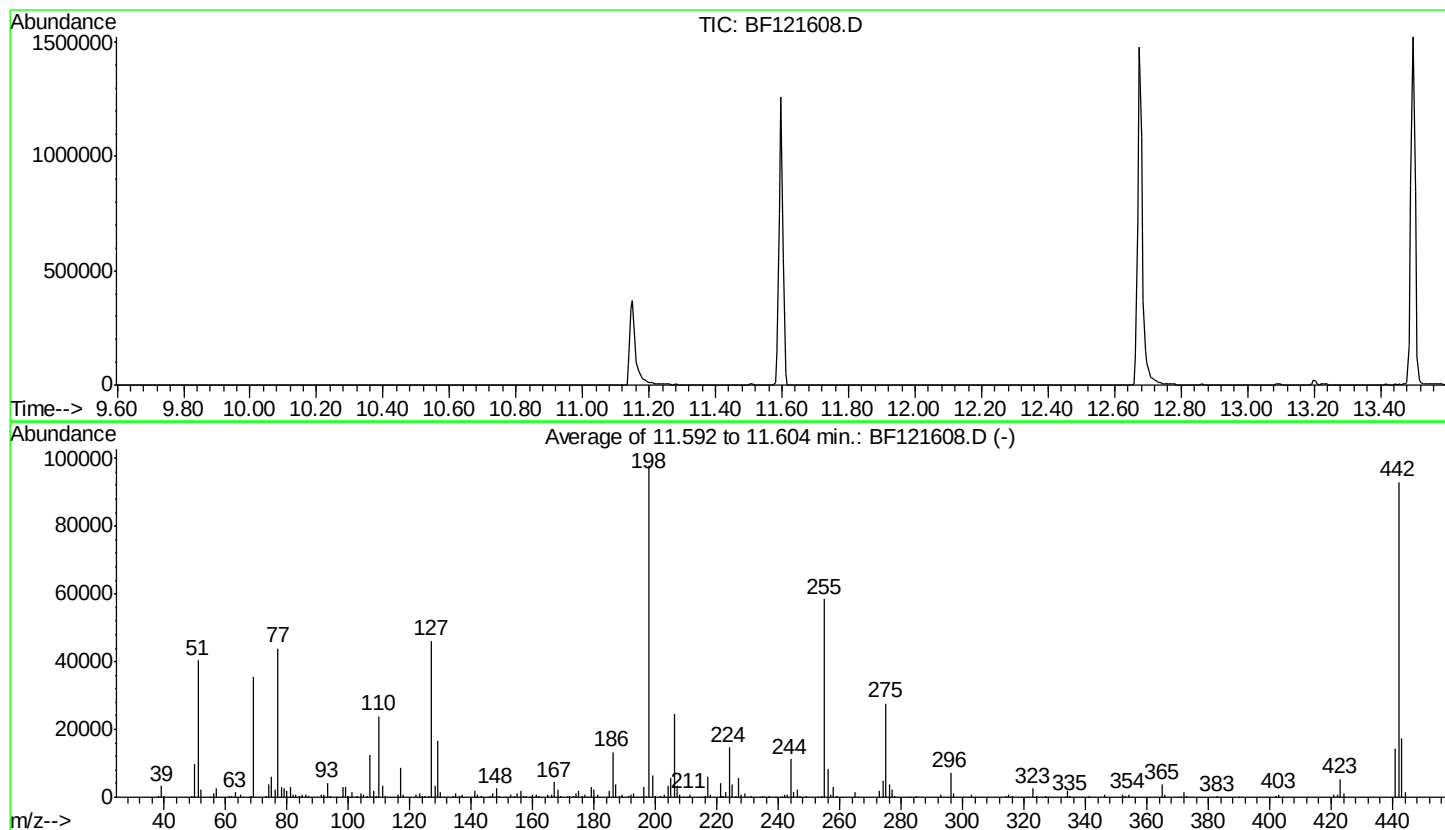

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	40390	PASS
68	69	0.00	2	1.6	563	PASS
69	198	0.00	100	36.2	35434	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	46280	PASS
197	198	0.00	2	0.5	496	PASS
198	198	100	100	100.0	97850	PASS
199	198	5	9	6.8	6620	PASS
275	198	10	60	28.3	27648	PASS
365	198	1	100	3.7	3665	PASS
441	198	0.01	100	14.6	14332	PASS
442	198	50	100	95.1	93048	PASS
443	442	15	24	18.7	17408	PASS