
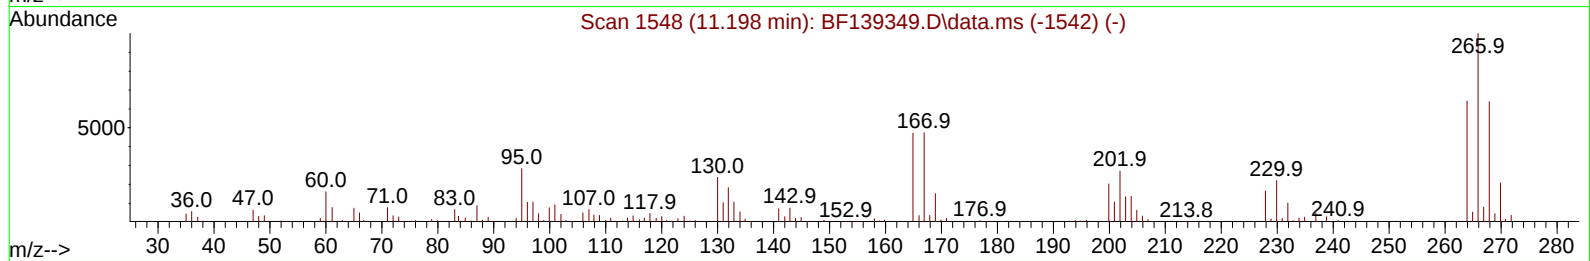
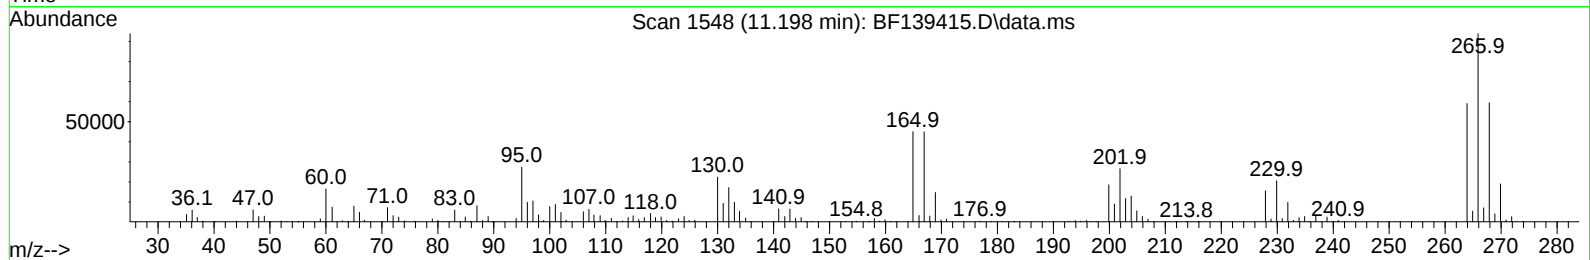


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091824\
Data File : BF139415.D
Acq On : 18 Sep 2024 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 11:16:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

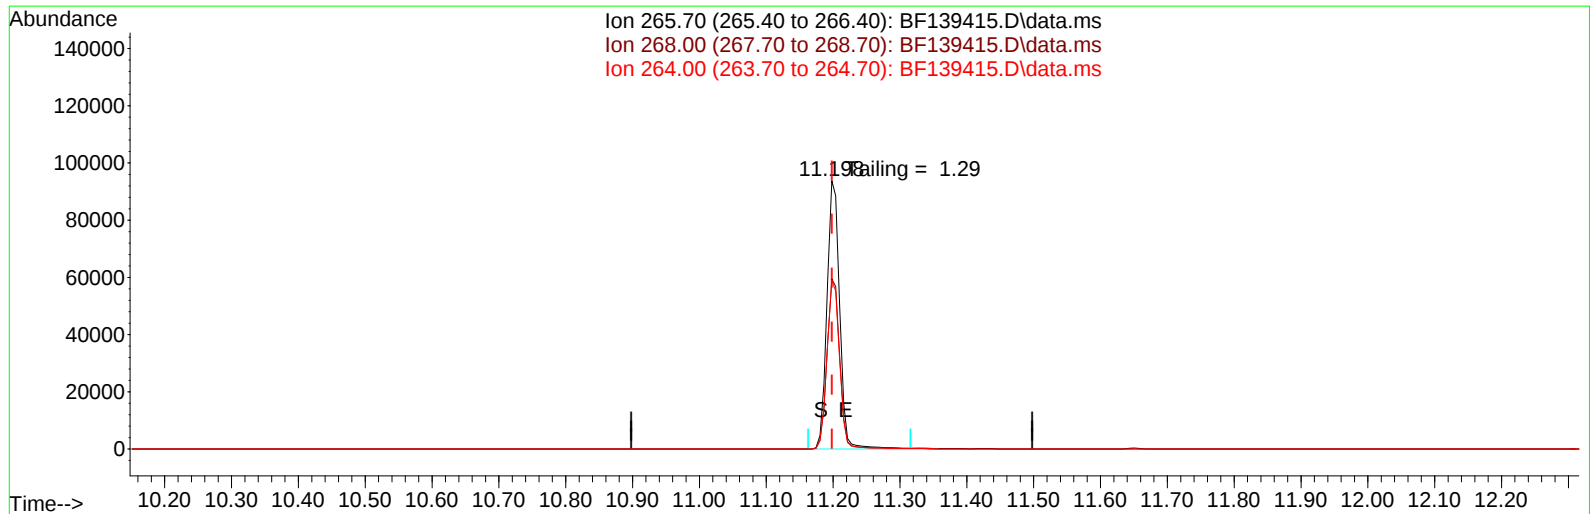

TIC: BF139415.D\data.ms

(70) Pentachlorophenol (C)




11.198min (-0.000) 32038.94 ng m

response 124763

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.40
264.00	64.20	62.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091824\
Data File : BF139415.D
Acq On : 18 Sep 2024 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 11:16:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

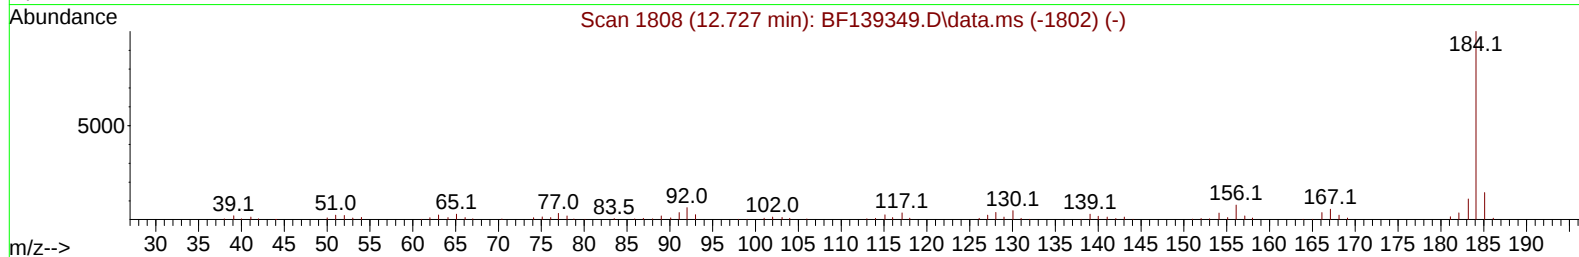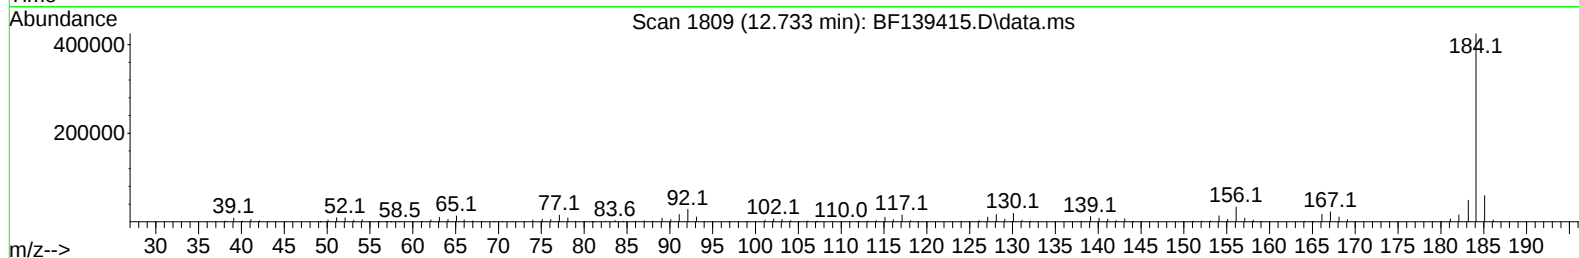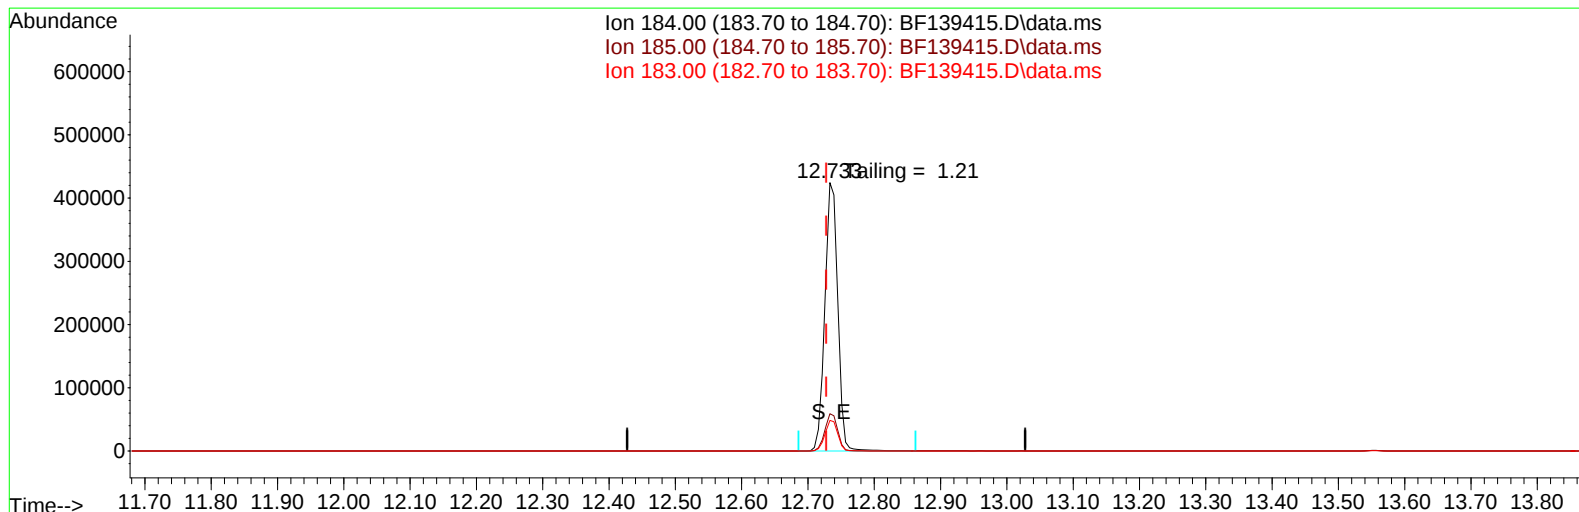

TIC: BF139415.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 0.00 ng

response 572592

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.88
183.00	11.10	11.41
0.00	0.00	0.00