
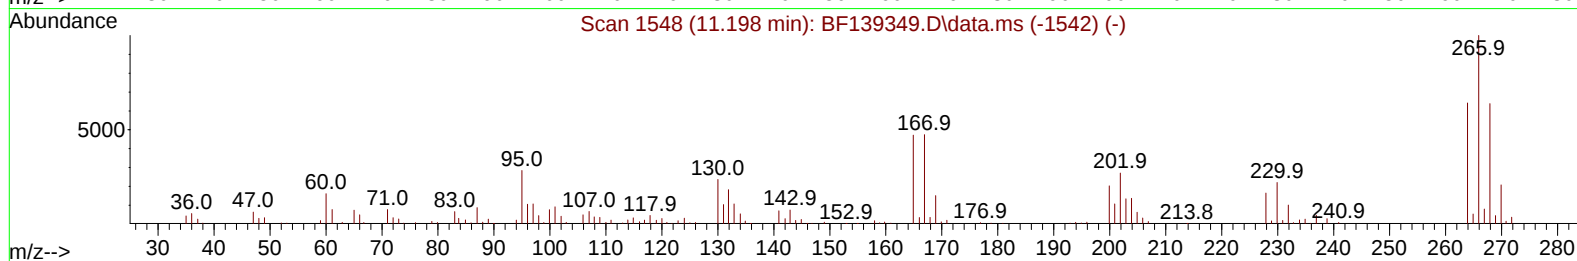
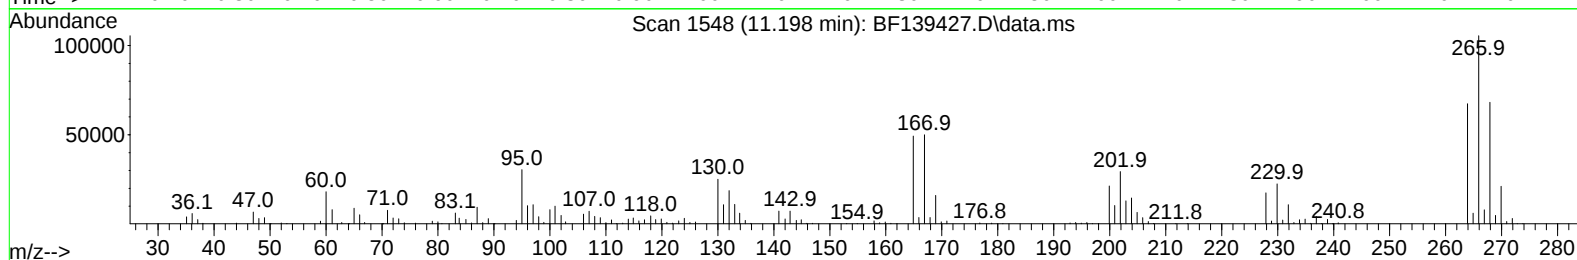


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091824\
Data File : BF139427.D
Acq On : 18 Sep 2024 15:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 16:54:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

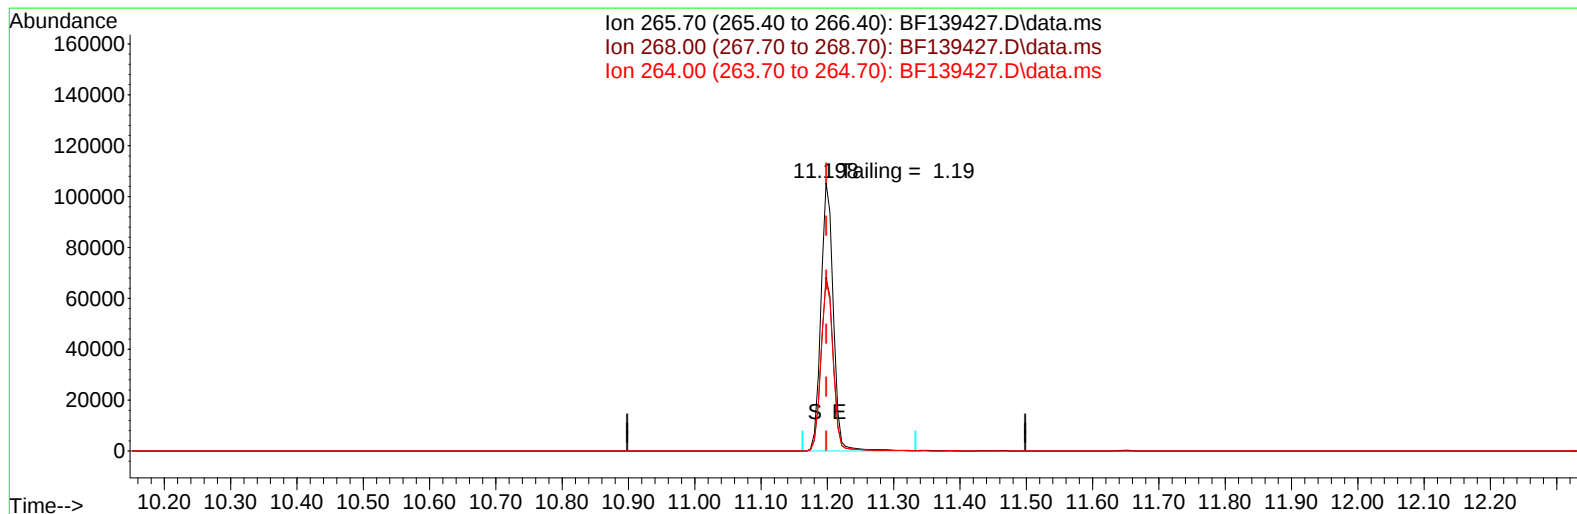

TIC: BF139427.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 85281.36 ng

response **137480**

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------




268.00	63.90	64.62
--------	-------	-------

264.00	64.20	63.86
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091824\
Data File : BF139427.D
Acq On : 18 Sep 2024 15:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 16:54:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

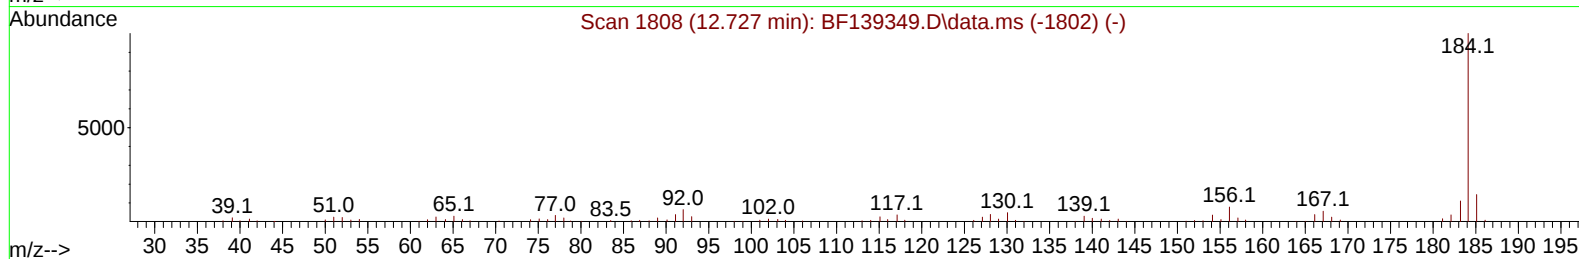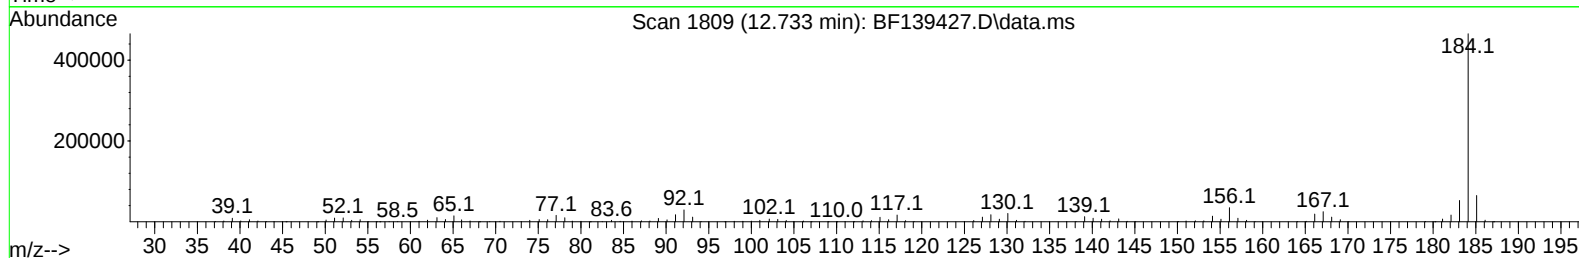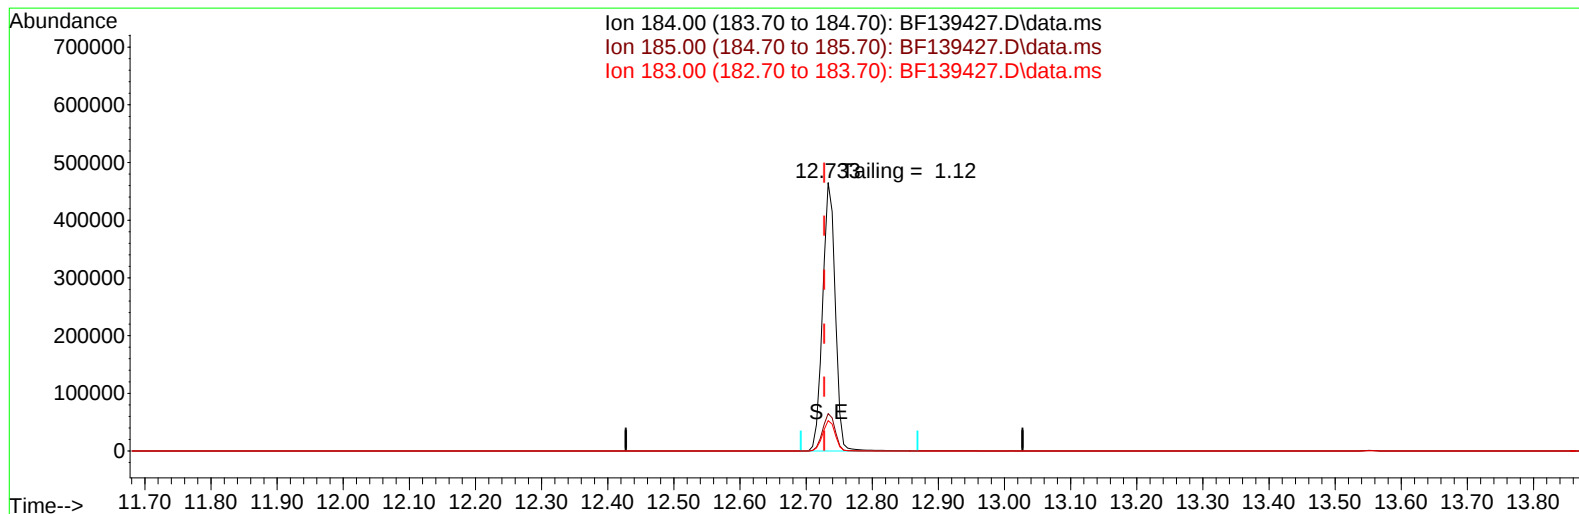

TIC: BF139427.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 341478.03 ng

response 616440

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.99
183.00	11.10	11.34
0.00	0.00	0.00