


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091824\
Data File : BF139415.D
Acq On : 18 Sep 2024 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 14 02:58:23 2024

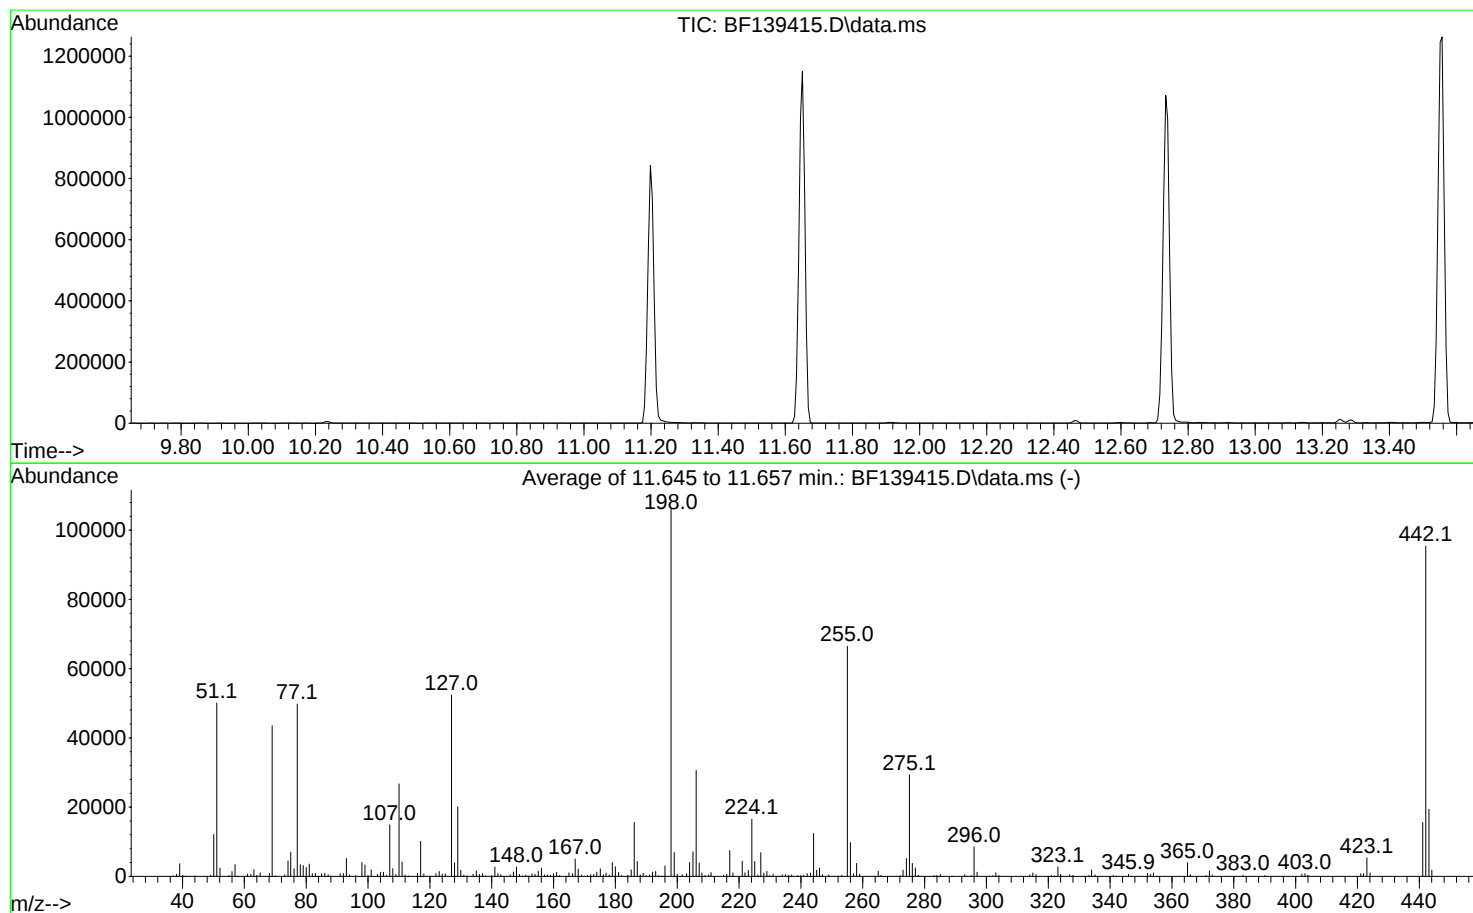




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	50109	PASS
68	69	0.00	2	2.0	869	PASS
69	198	0.00	100	40.9	43507	PASS
70	69	0.00	2	0.4	161	PASS
127	198	10	80	49.3	52349	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	106261	PASS
199	198	5	9	6.5	6888	PASS
275	198	10	60	27.6	29357	PASS
365	198	1	100	3.7	3930	PASS
441	198	0.01	100	14.7	15599	PASS
442	442	50	100	100.0	95400	PASS
443	442	15	24	20.3	19388	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091824\
Data File : BF139415.D
Acq On : 18 Sep 2024 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 18 11:16:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

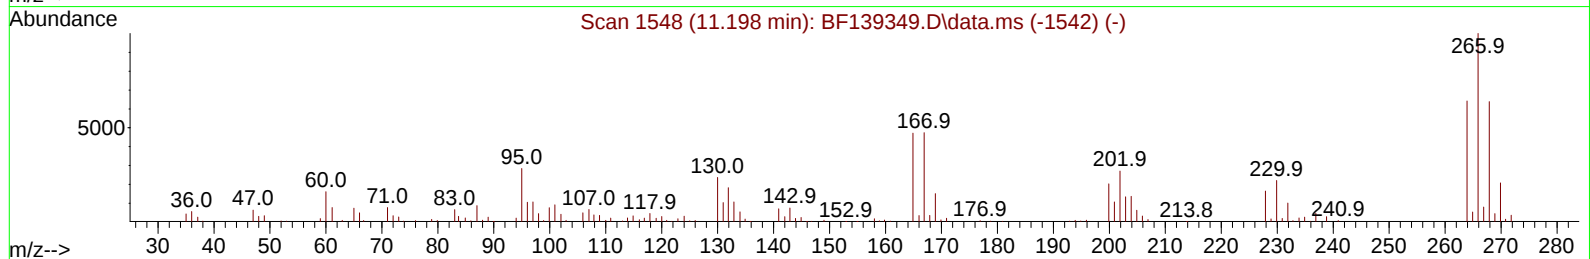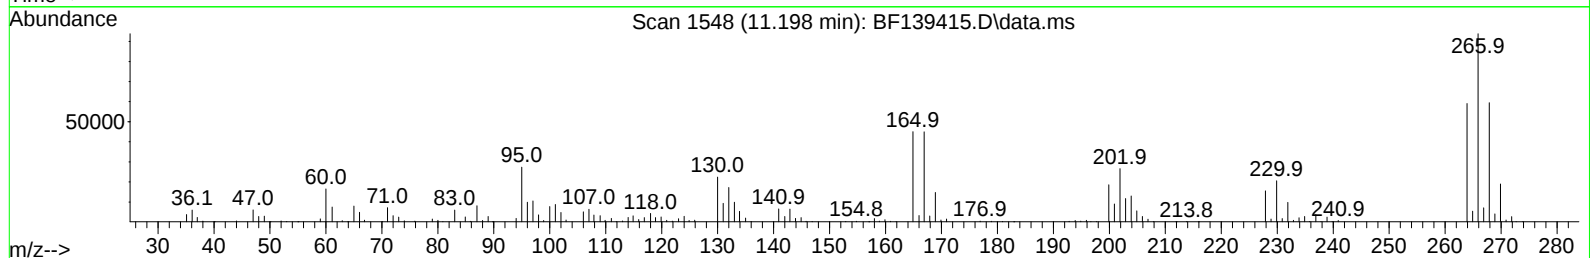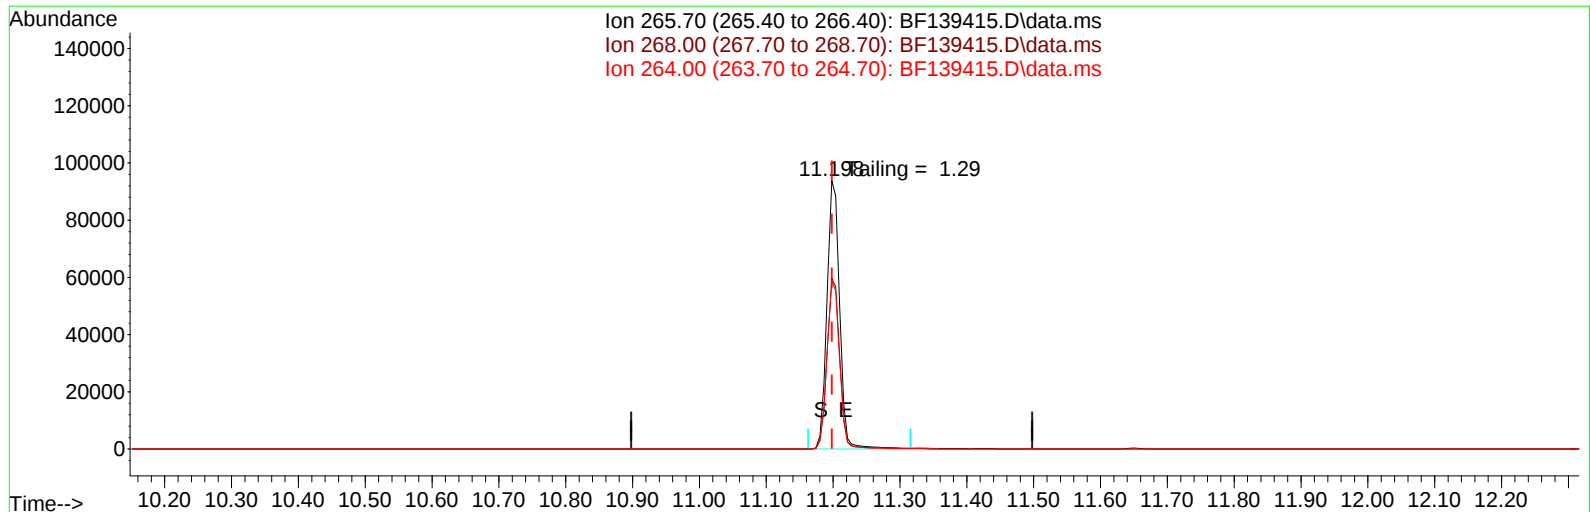

TIC: BF139415.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 32038.94 ng m




response 124763

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.40
264.00	64.20	62.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091824\
Data File : BF139415.D
Acq On : 18 Sep 2024 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 18 11:16:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

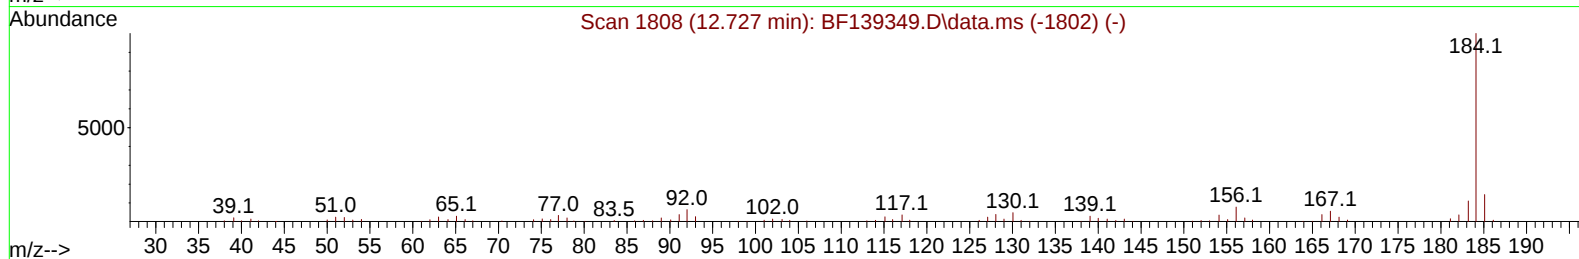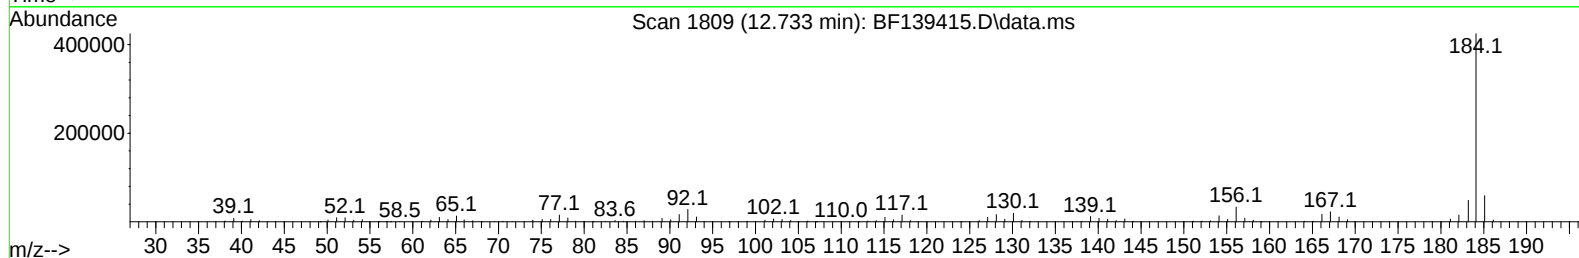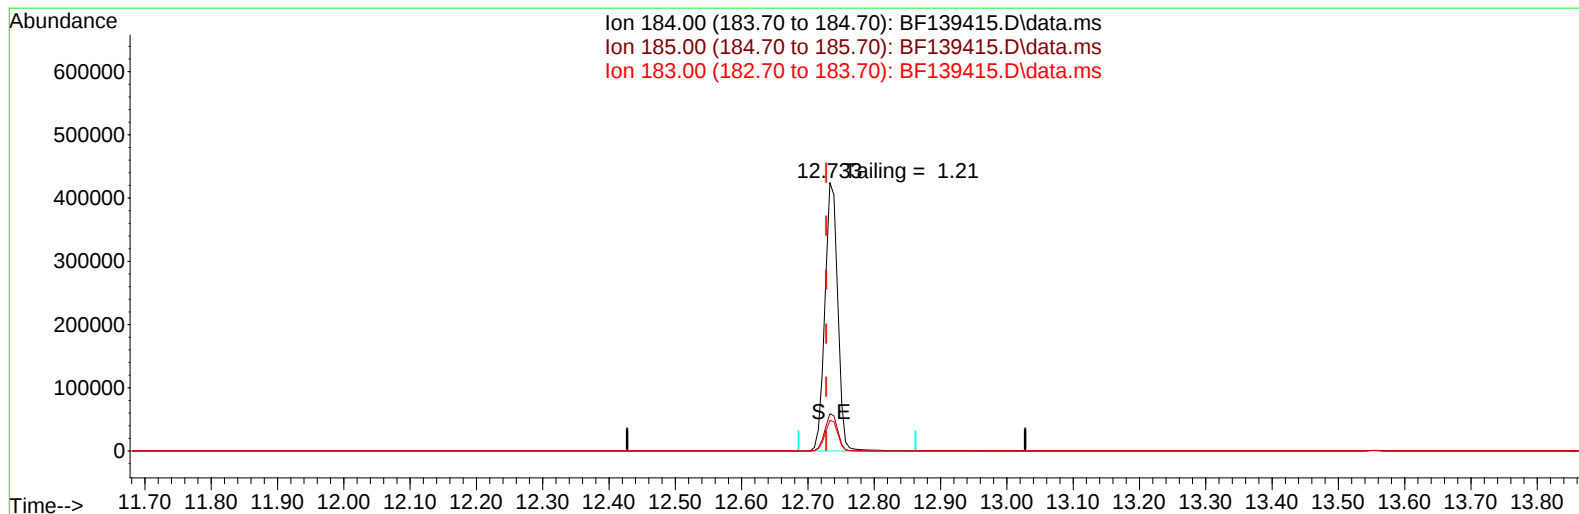

TIC: BF139415.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 0.00 ng

response 572592

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.88
183.00	11.10	11.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/18/2024	BNA_F	<u>BF139415.D</u>
Compound Name	Response	Retention Time
DDT	311181	13.557
DDD	6253	13.257
DDE	361	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6614	317795	2.08

P

Instrument :
BNA_F
ClientSampleId :
DFTPP