

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091916\
 Data File : BF090126.D
 Acq On : 19 Sep 2016 18:09
 Operator : UM/SJ
 Sample : H4840-01 20X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FILL-1-SOILPILE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.690	7	9	41	rVB	730345	1709626	100.00%	22.354%
2	5.107	305	308	313	rBV	8154	17757	1.04%	0.232%
3	6.193	400	403	407	rBV	10079	19447	1.14%	0.254%
4	6.296	411	412	418	rVB2	17671	26179	1.53%	0.342%
5	6.536	430	433	435	rBV	539586	750734	43.91%	9.816%
6	6.685	444	446	453	rVB	31342	32874	1.92%	0.430%
7	7.816	543	545	548	rBV	1048229	1032182	60.37%	13.496%
8	8.902	638	640	642	rBV	37781	37024	2.17%	0.484%
9	9.565	695	698	700	rBV	1421015	1208037	70.66%	15.795%
10	10.616	789	790	794	rVB	10226	17181	1.00%	0.225%
11	11.028	824	826	829	rBV	897280	951593	55.66%	12.442%
12	12.468	949	952	953	rBV	12900	18432	1.08%	0.241%
13	12.617	963	965	967	rBV	19691	29576	1.73%	0.387%
14	13.542	1043	1046	1049	rBV	24825	39283	2.30%	0.514%
15	13.645	1052	1055	1057	rBV	766004	849249	49.67%	11.104%
16	14.160	1098	1100	1102	rBV	15809	18571	1.09%	0.243%
17	14.971	1168	1171	1174	rBV	738997	831332	48.63%	10.870%
18	15.394	1206	1208	1210	rBV	38568	58957	3.45%	0.771%


Sum of corrected areas: 7648034

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091916\
Data File : BF090126.D
Acq On : 19 Sep 2016 18:09
Operator : UM/SJ
Sample : H4840-01 20X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FILL-1-SOILPILE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

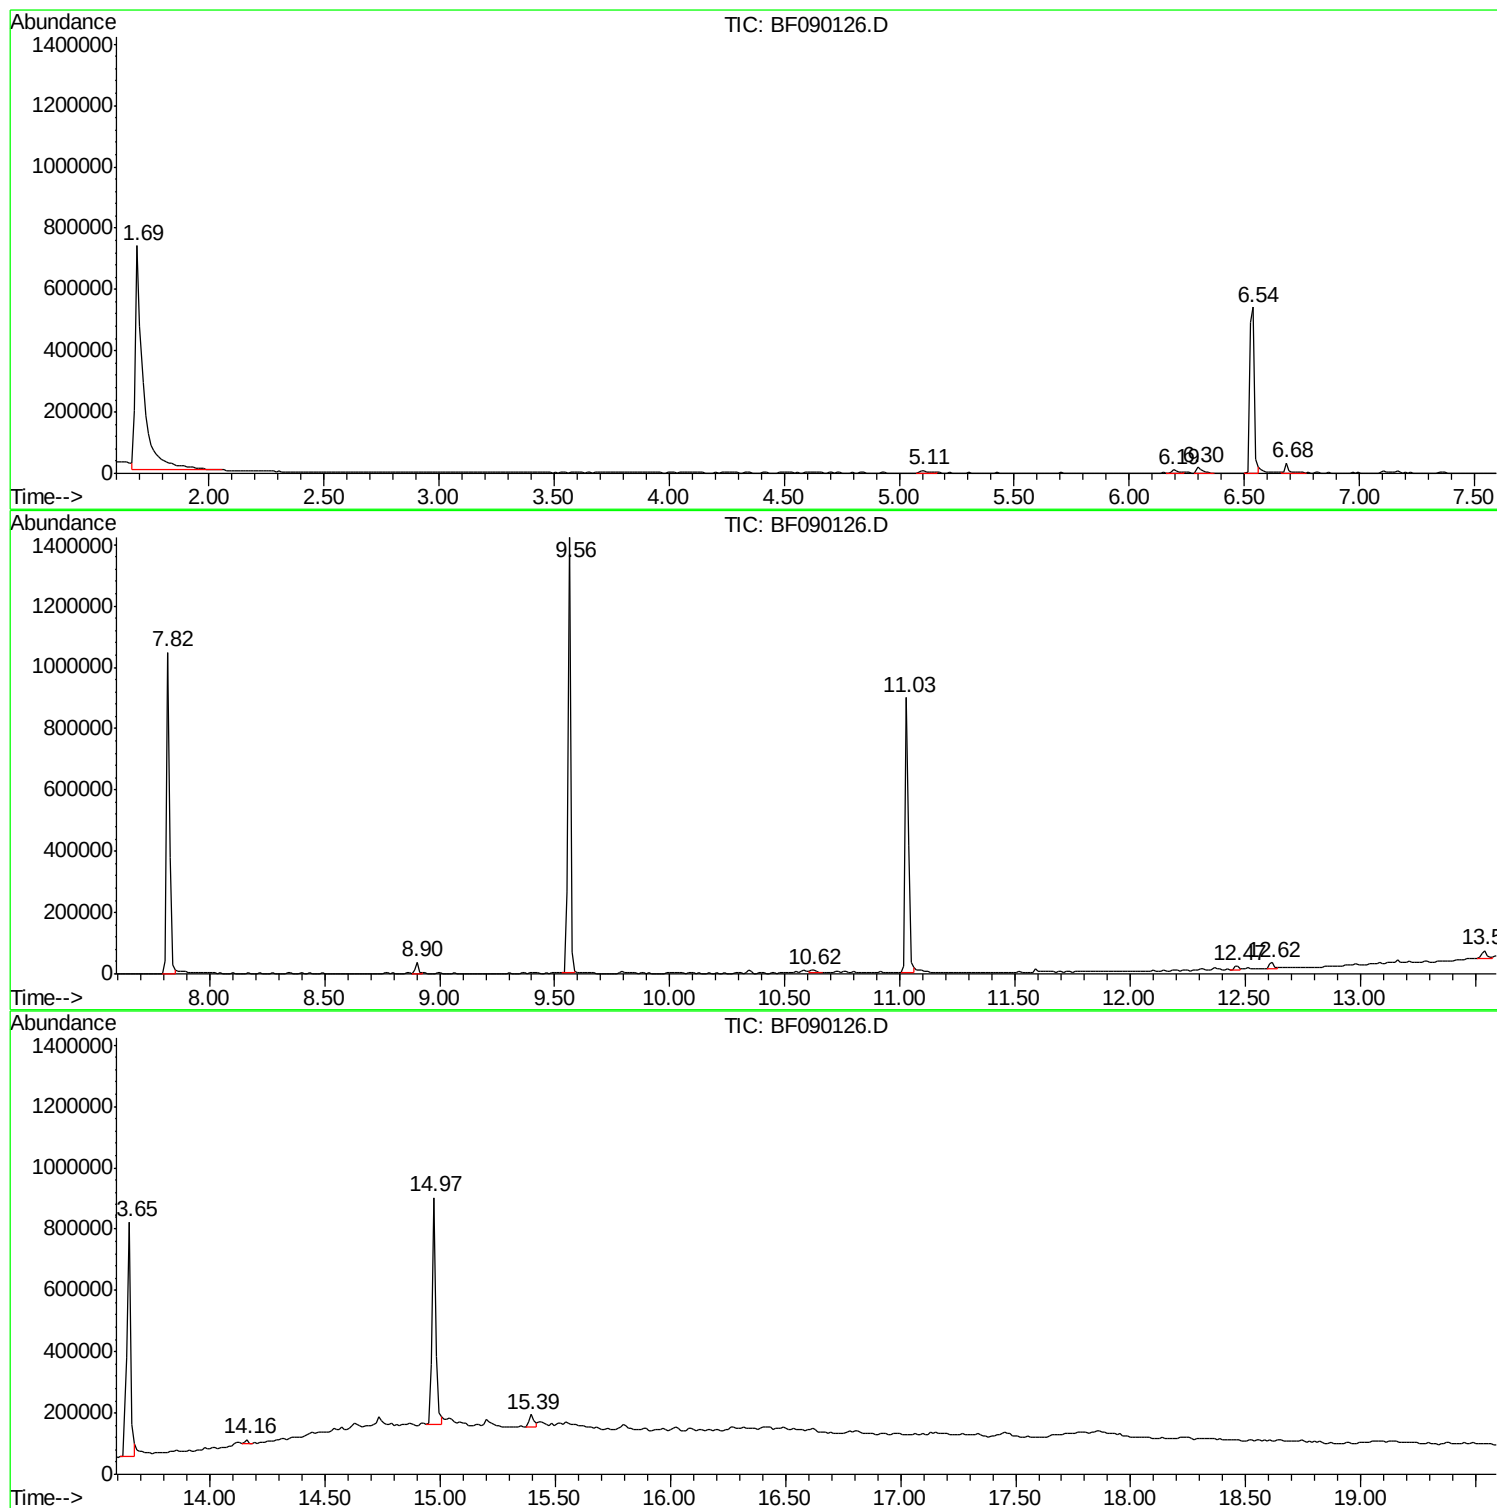

DbaaaPbath::ZZ\NRPBHHM1BBAFNDATA\BB00000066\
 DbaaaFile::BB0000206DD
 Aeqq00n ::109S8pp20066 188009
 Oppaaaor ::UMMSJ
 Samplee ::H43300001200X
 Misc ::
 AASSVaal ::77 SampleeMMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 FILL-1-SOILPILE

QqaabtMebbdd::ZZ\NRPBHHM1BBAFMEH00S88200BB0005566MM
 QqaabtTitle ::ASBPBBAASSANDBBSF00R55P000NTCALIBRATION

TICCLibbaay ::CC\NbaaaabaaeN0\$ST11LL
 TICInteggaafionPbaaaeeess:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	-Internal Standard-
				#	RT Resp Conc

No Library Search Compounds Detected
