
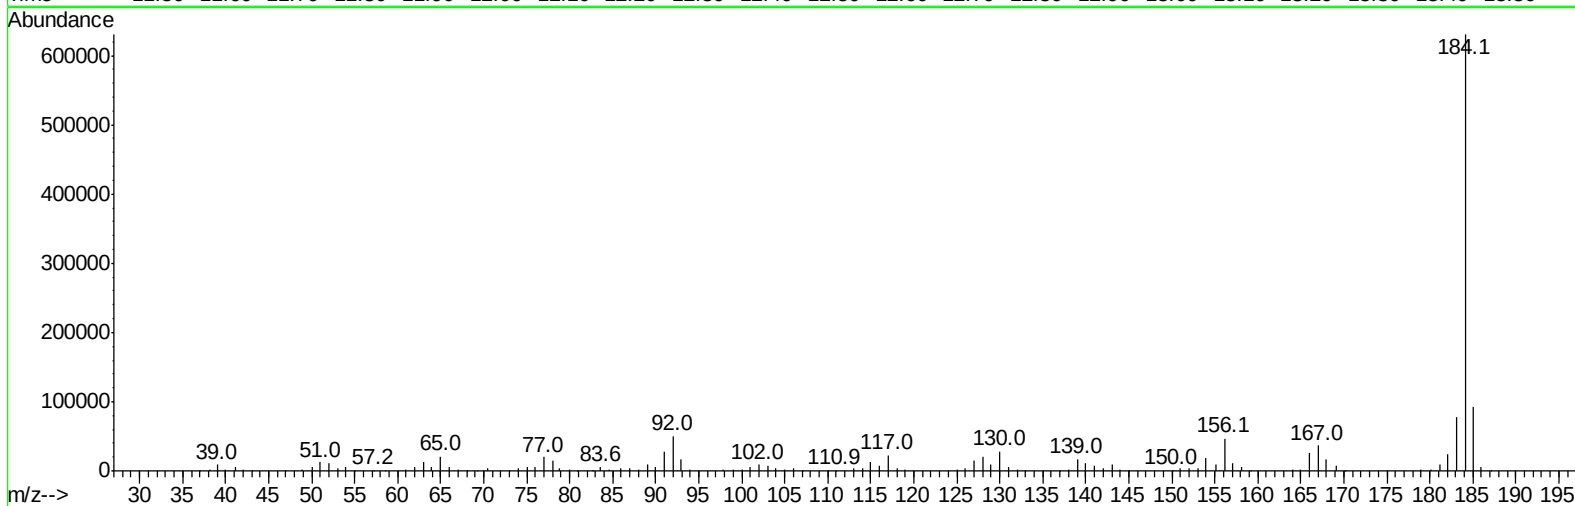


Data Path : Z:\HPCHEM1\BNA F\Data\BF091917\
Data File : BF098637.D
Acq On : 19 Sep 2017 12:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 08:30:57 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 18 13:37:24 2017
Response via : Initial Calibration

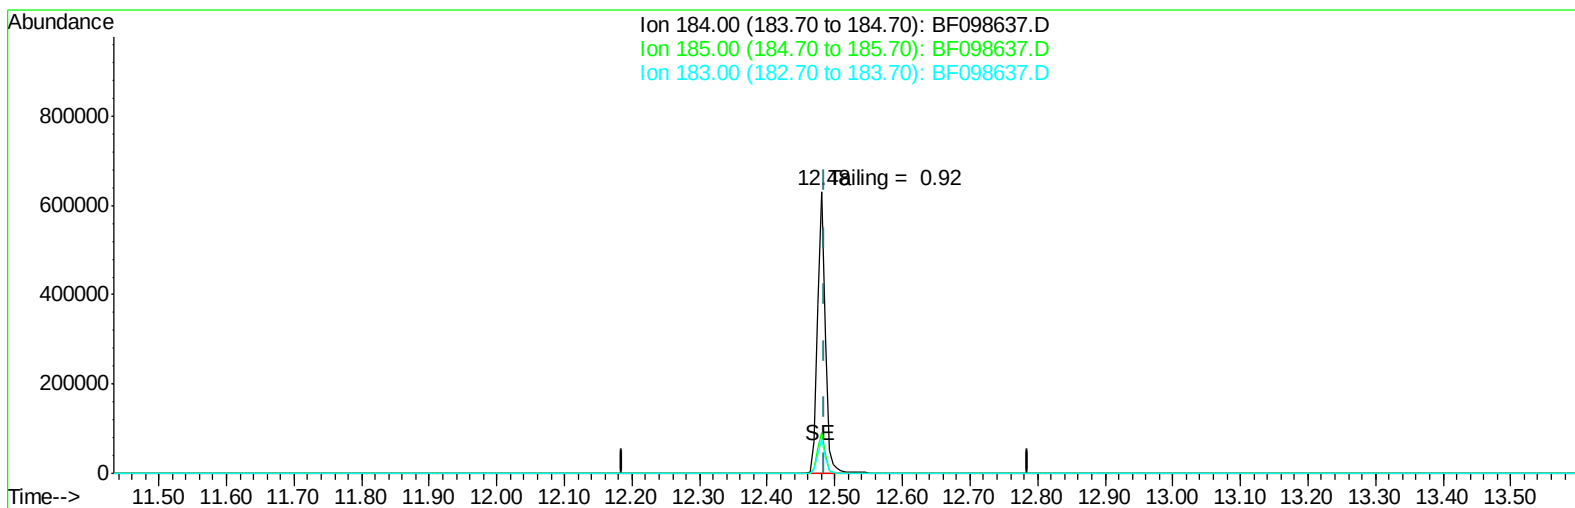

TIC: BF098637.D

(76) Benzidine



12.480min (-0.006) 0.00ng

response 527301

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.77#
183.00	12.20	12.32
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF091917\
Data File : BF098637.D
Acq On : 19 Sep 2017 12:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 08:30:57 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 18 13:37:24 2017
Response via : Initial Calibration

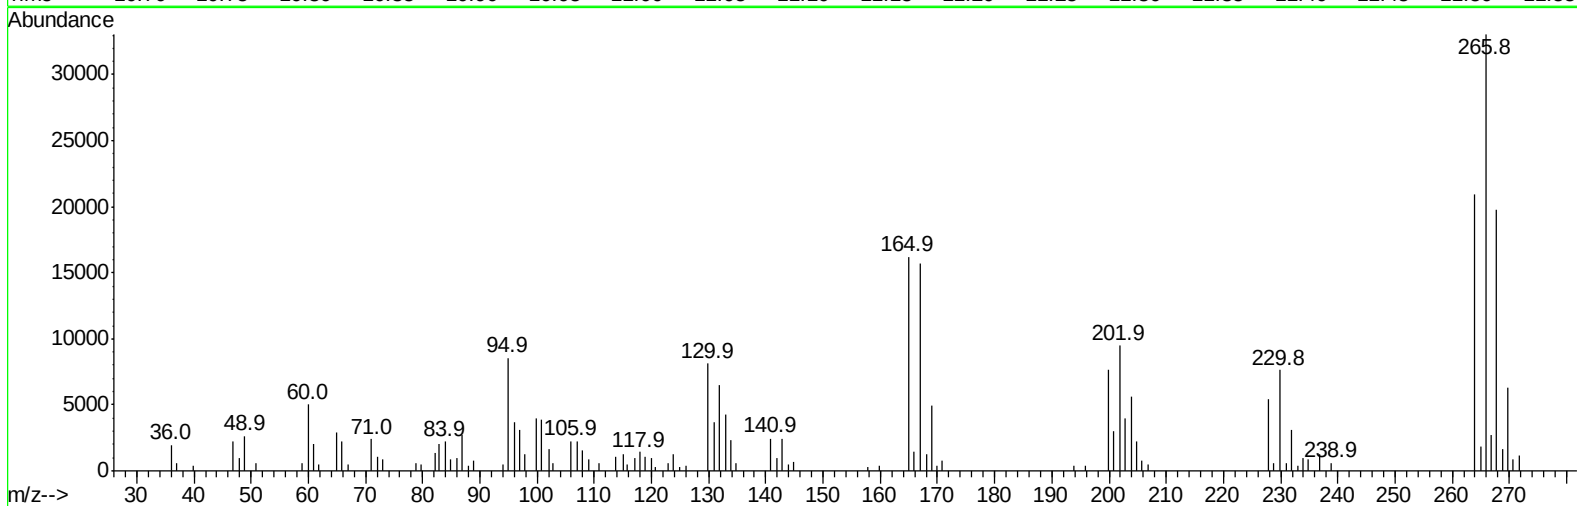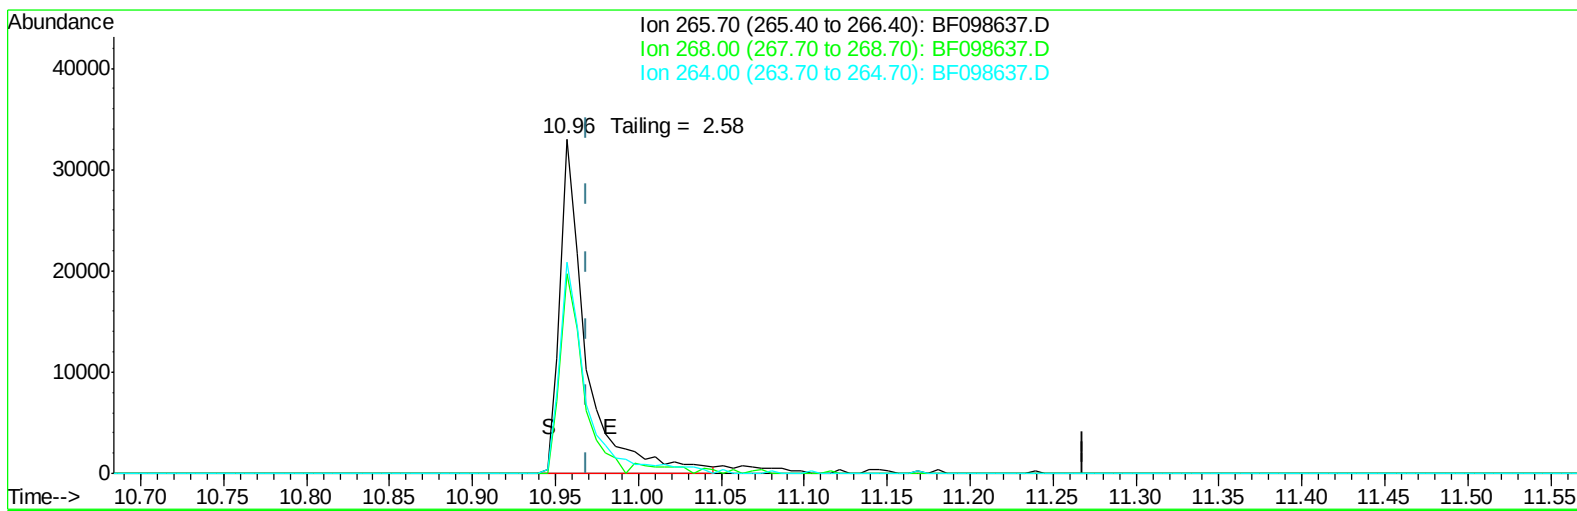

TIC: BF098637.D

(69) Pentachlorophenol (C)

10.957min (-0.012) 25501.30ng

response 37830

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.74
264.00	64.60	63.23
0.00	0.00	0.00