

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091917\
 Data File : BF098643.D
 Acq On : 19 Sep 2017 16:09
 Operator : SJ/JU
 Sample : PB102430TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB102430TB

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.822	461	465	480	rBV	336128	564865	12.34%	1.604%
2	5.246	533	537	559	rBV	3670969	3689797	80.58%	10.480%
3	6.281	708	713	716	rBV	3107410	3551597	77.56%	10.087%
4	6.398	729	733	736	rBV	3939087	3571915	78.00%	10.145%
5	6.622	768	771	783	rVB	913287	799591	17.46%	2.271%
6	6.781	794	798	801	rBV	3096195	2770484	60.50%	7.869%
7	7.198	864	869	872	rBV	2077473	2123072	46.36%	6.030%
8	7.910	985	990	998	rBV	1048589	1057300	23.09%	3.003%
9	8.986	1167	1173	1176	rBV	3937301	3905931	85.30%	11.094%
10	9.657	1282	1287	1294	rVB	1328677	1260265	27.52%	3.579%
11	10.451	1416	1422	1425	rBV	2629150	2557638	55.85%	7.264%
12	11.139	1534	1539	1543	rBV	1634297	1472047	32.15%	4.181%
13	12.727	1802	1809	1812	rBV	3951225	4579087	100.00%	13.006%
14	13.774	1983	1987	1994	rVB	1535161	1531121	33.44%	4.349%
15	15.174	2219	2225	2237	rVB	1269742	1521902	33.24%	4.323%
16	15.563	2286	2291	2296	rVB	40729	57345	1.25%	0.163%
17	16.010	2362	2367	2372	rBV2	44207	68394	1.49%	0.194%
18	16.527	2449	2455	2462	rVB4	30286	62207	1.36%	0.177%
19	17.133	2552	2558	2566	rVB5	27709	63784	1.39%	0.181%


Sum of corrected areas: 35208342

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091917\
Data File : BF098643.D
Acq On : 19 Sep 2017 16:09
Operator : SJ/JU
Sample : PB102430TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB102430TB

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

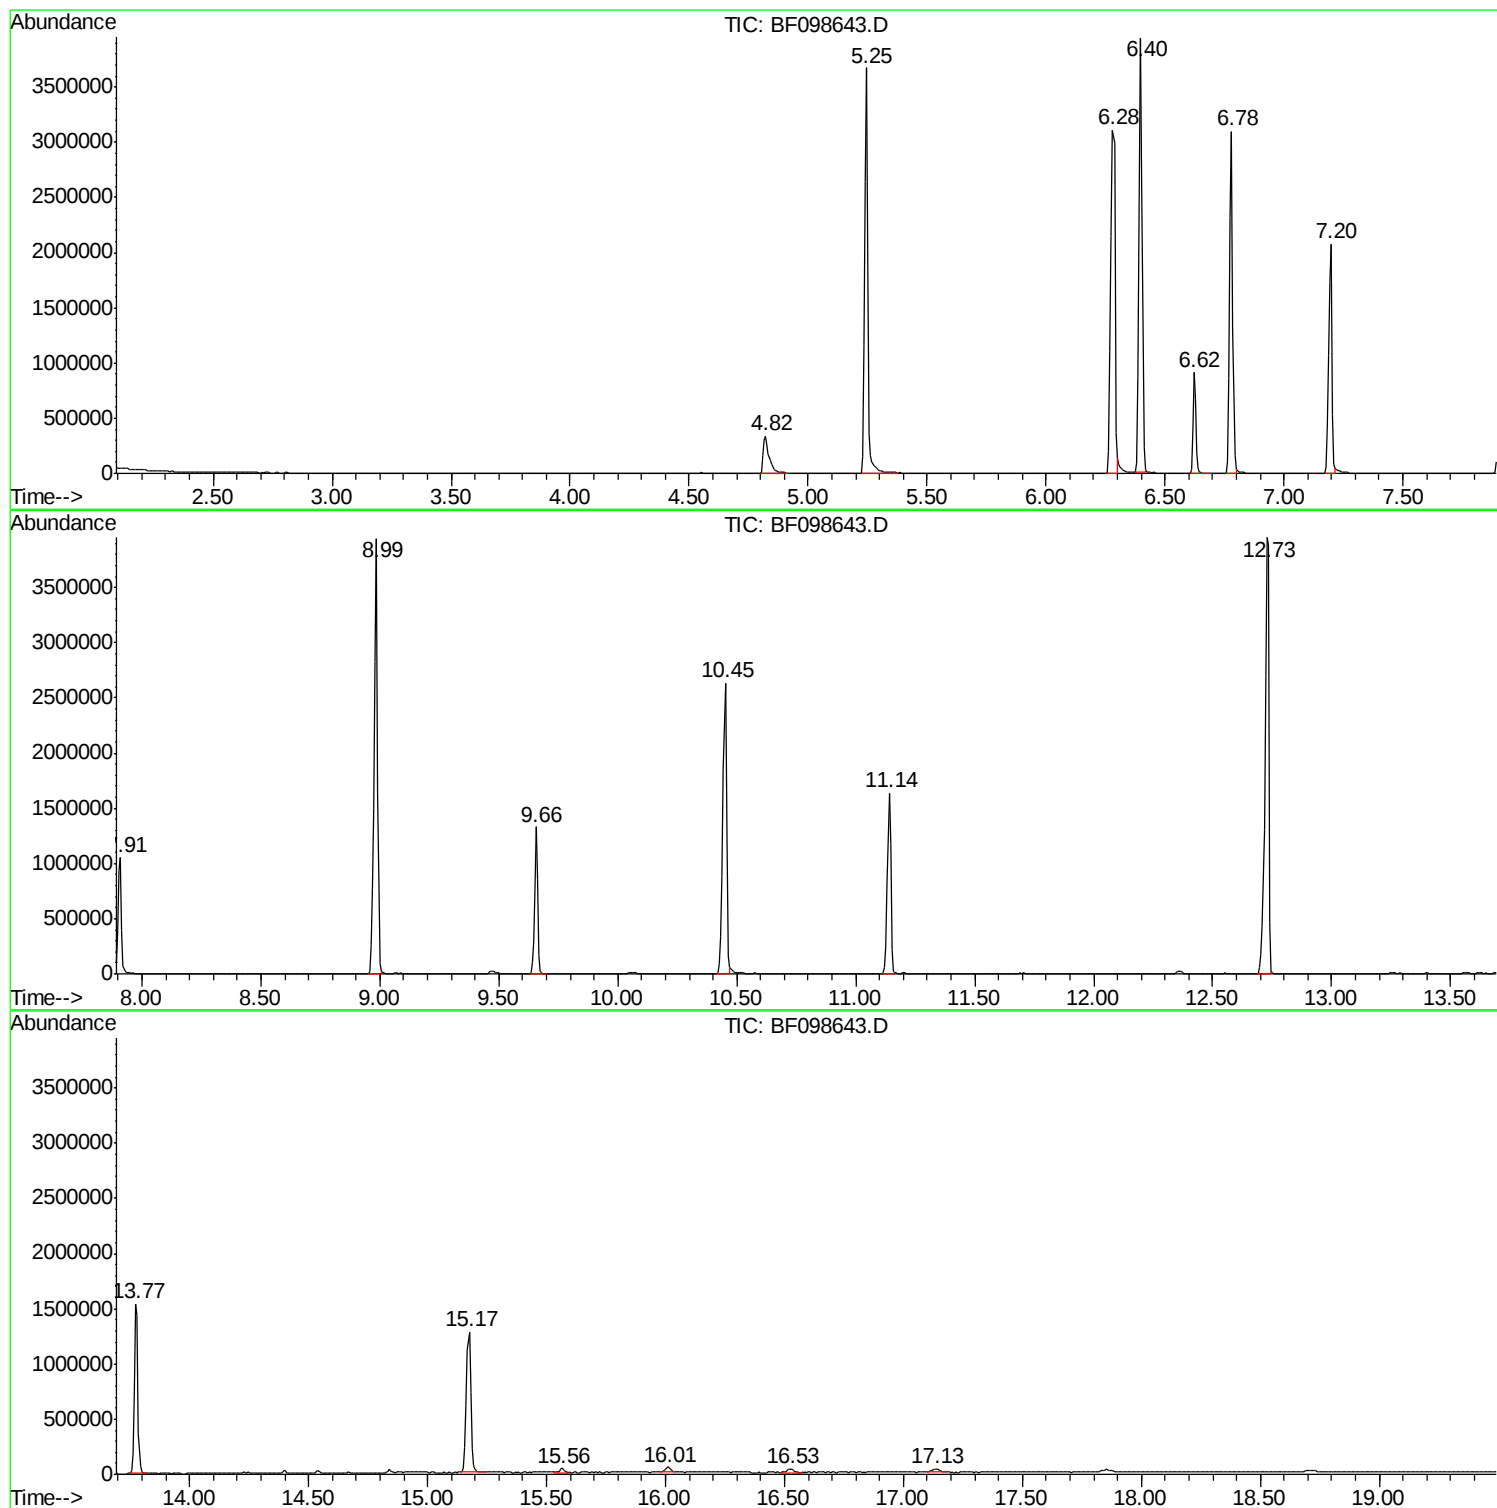

DbaaaPbath::ZZ\NRPBEMM1BBAFNDAAABBB0000IX\
 DbaaaFile::BB000003DD
 AaqQOn ::109Spp2007 166009
 Opeaaor ::SSJUU
 Sample ::PB000230TB
 Misc ::
 AASSVal ::77 SampleMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 PB102430TB

QqaabMebdd::ZZ\NRPBEMM1BBAFMEH00S8200BB00117MM
 QqaabFile ::ASBPBNASSANDABBSF00R55P000NTCALIBRATION

TICLibbaay ::CC\DAABASSEN0\$T11LL
 TICIntegratioonParameters:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
