


Data Path : Z:\HPCHEM1\BNA_F\Data\BF091917\
 Data File : BF098637.D
 Acq On : 19 Sep 2017 12:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 18 13:37:24 2017

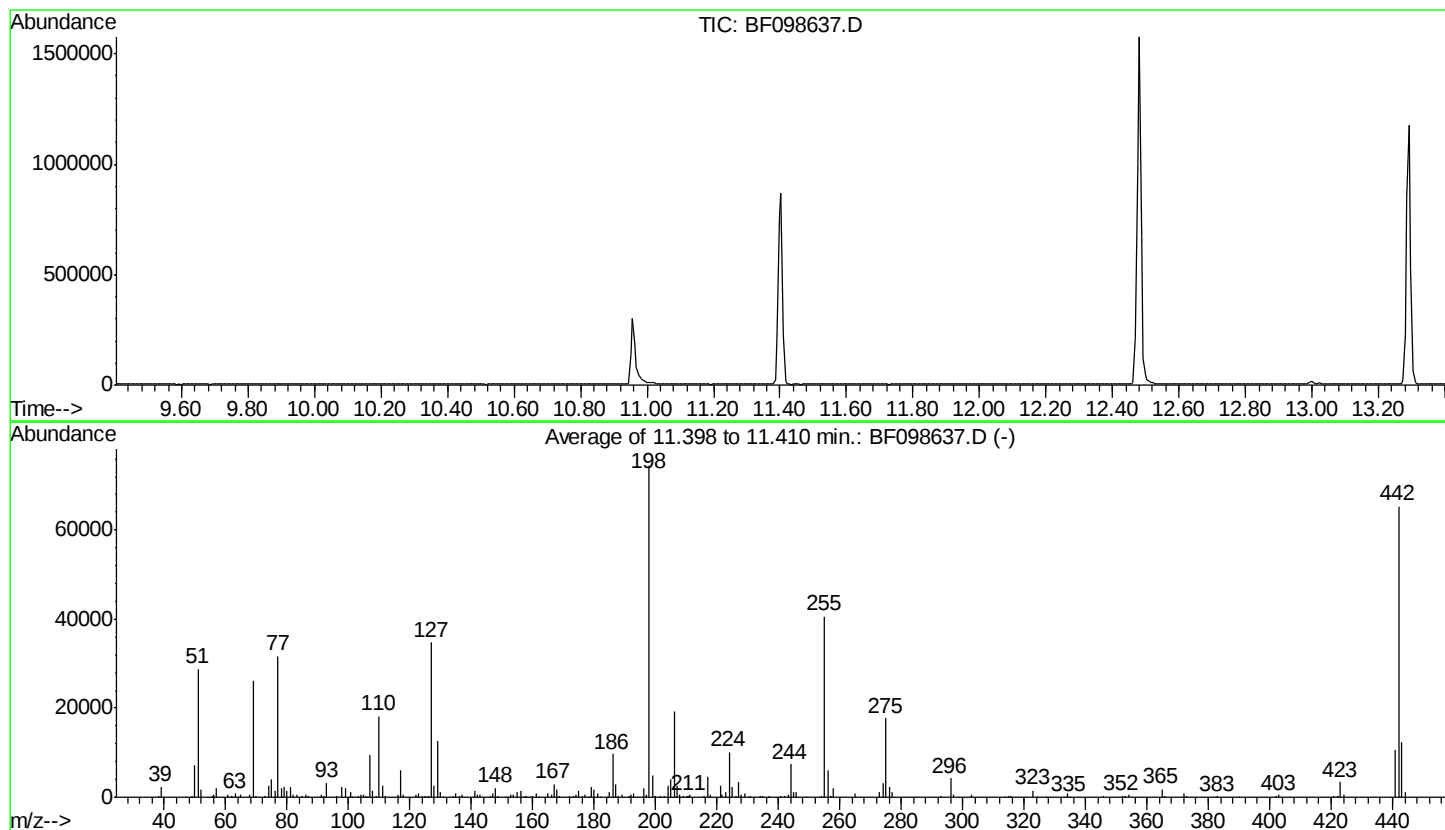

AutoFind: Scans 1583, 1584, 1585; Background Corrected with Scan 1577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	28890	PASS
68	69	0.00	2	1.8	482	PASS
69	198	0.00	100	35.2	26181	PASS
70	69	0.00	2	0.8	200	PASS
127	198	10	80	46.7	34759	PASS
197	198	0.00	2	0.7	516	PASS
198	198	100	100	100.0	74456	PASS
199	198	5	9	6.6	4889	PASS
275	198	10	60	23.8	17714	PASS
365	198	1	100	2.4	1791	PASS
441	442	0.01	24	16.4	10695	PASS
442	198	50	100	87.7	65277	PASS
443	442	15	24	18.9	12334	PASS