
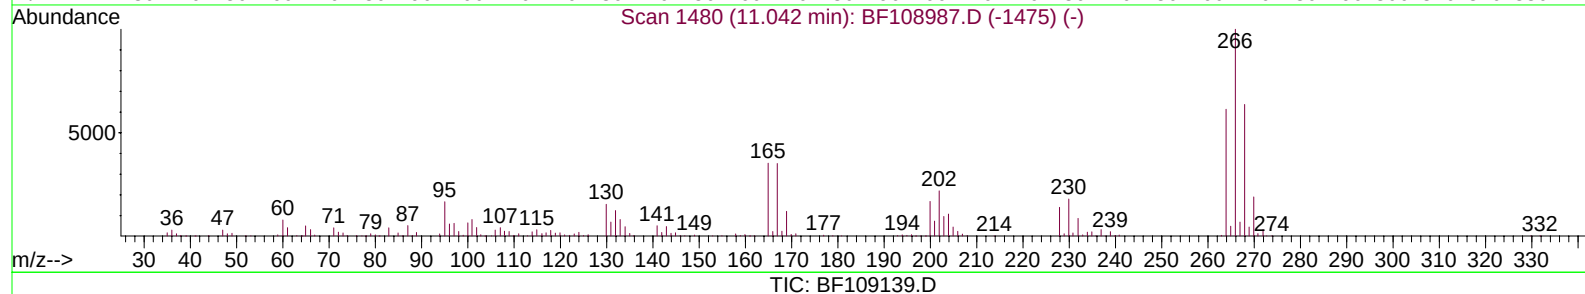
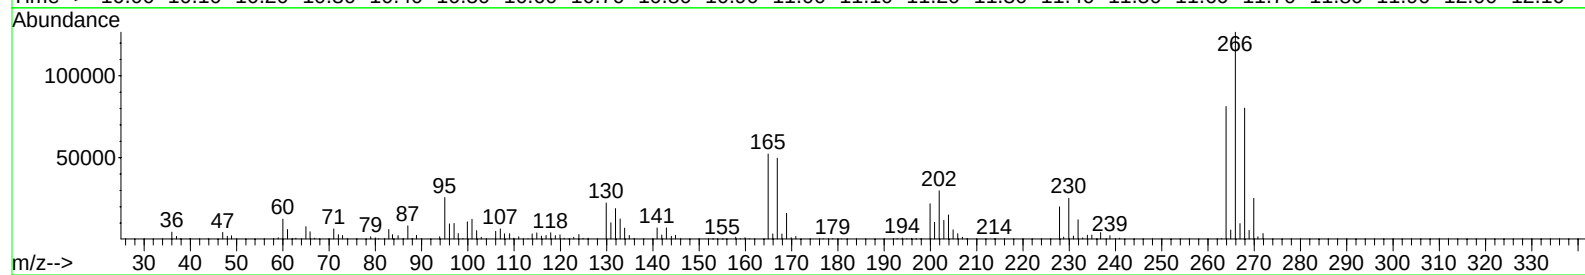


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091918\
 Data File : BF109139.D
 Acq On : 19 Sep 2018 13:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 16:28:48 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 14 13:26:52 2018
 Response via : Initial Calibration

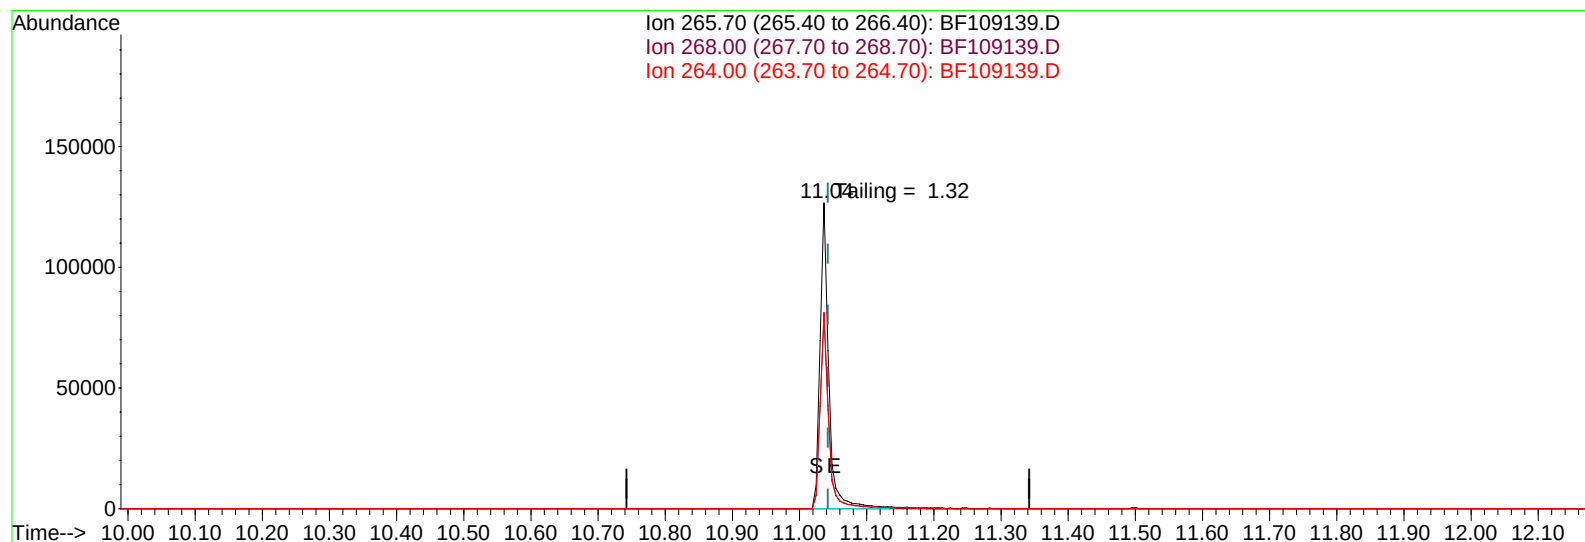

(69) Pentachlorophenol (C)




11.036min (-0.006) 27514.11ng

response 115902

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.43
264.00	61.90	64.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091918\
Data File : BF109139.D
Acq On : 19 Sep 2018 13:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 16:28:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 14 13:26:52 2018
Response via : Initial Calibration

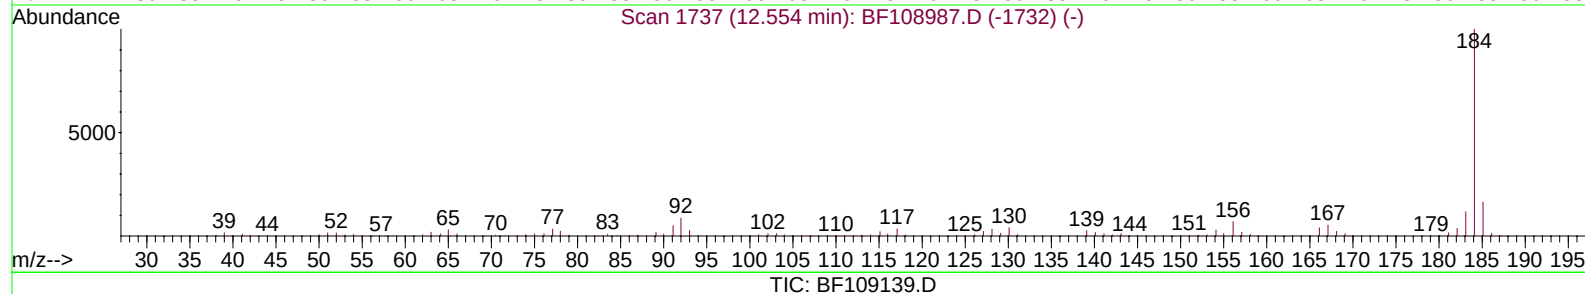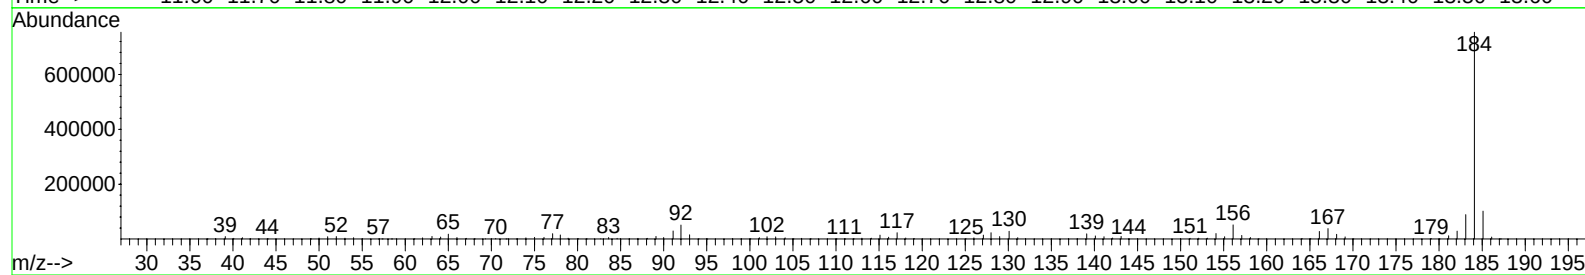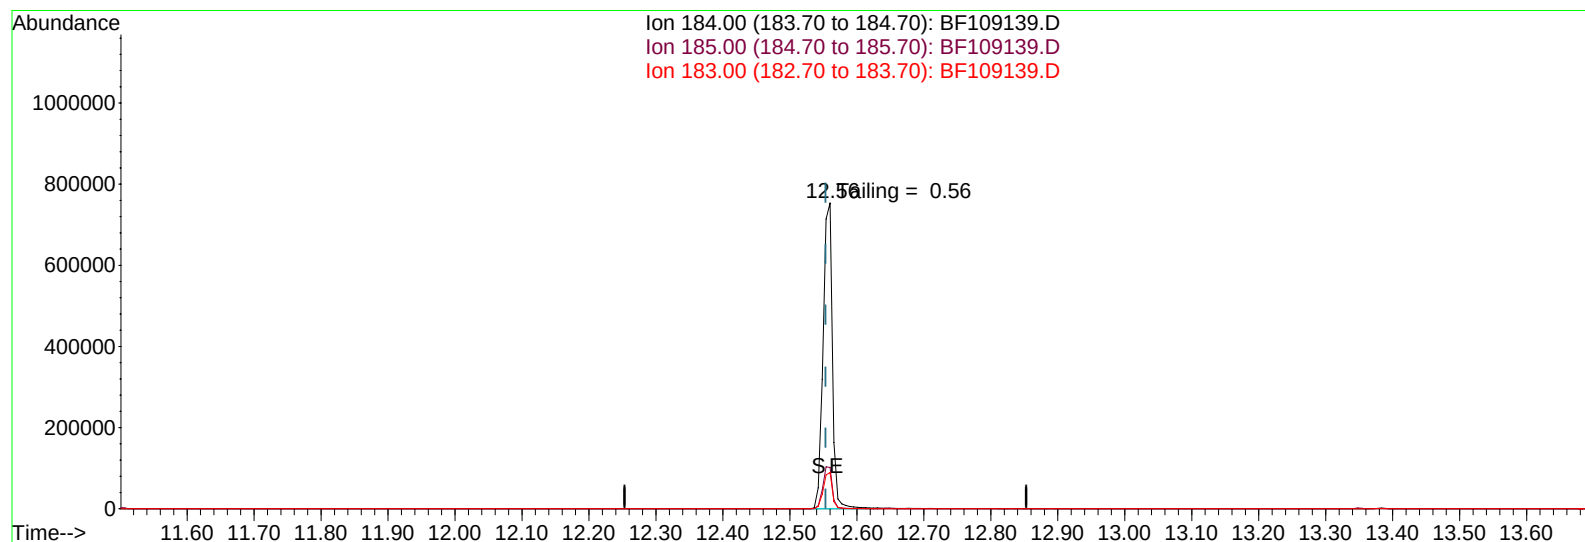

(76) Benzidine

12.560min (+0.007) 0.00ng

response 735478

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.53
183.00	11.60	11.84
0.00	0.00	0.00