

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091918\
 Data File : BF109171.D
 Acq On : 20 Sep 2018 3:43
 Operator : JU/SJ
 Sample : J4984-09
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 091718-TIPC-E-D-M

Quant Time: Sep 20 08:31:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 14 13:26:52 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.72	152	136443	20.00	ng	0.00
21) Naphthalene-d8	8.00	136	481379	20.00	ng	0.00
38) Acenaphthene-d10	9.75	164	194036	20.00	ng	0.00
63) Phenanthrene-d10	11.22	188	328568	20.00	ng	0.00
75) Chrysene-d12	13.85	240	337661	20.00	ng	-0.01
86) Perylene-d12	15.25	264	301628	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	325386	39.61	ng	0.00
7) Phenol-d6	6.35	99	256213	24.19	ng	-0.01
23) Nitrobenzene-d5	7.28	82	744896	86.79	ng	0.00
41) 2,4,6-Tribromophenol	10.53	330	144218	68.49	ng	-0.01
44) 2-Fluorobiphenyl	9.08	172	1228830	99.22	ng	0.00
78) Terphenyl-d14	12.81	244	1117813	78.47	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.47	163	69040	4.978	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091918\
Data File : BF109171.D
Acq On : 20 Sep 2018 3:43
Operator : JU/SJ
Sample : J4984-09
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
091718-TIPC-E-D-M

Quant Time: Sep 20 08:31:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 14 13:26:52 2018
Response via : Initial Calibration

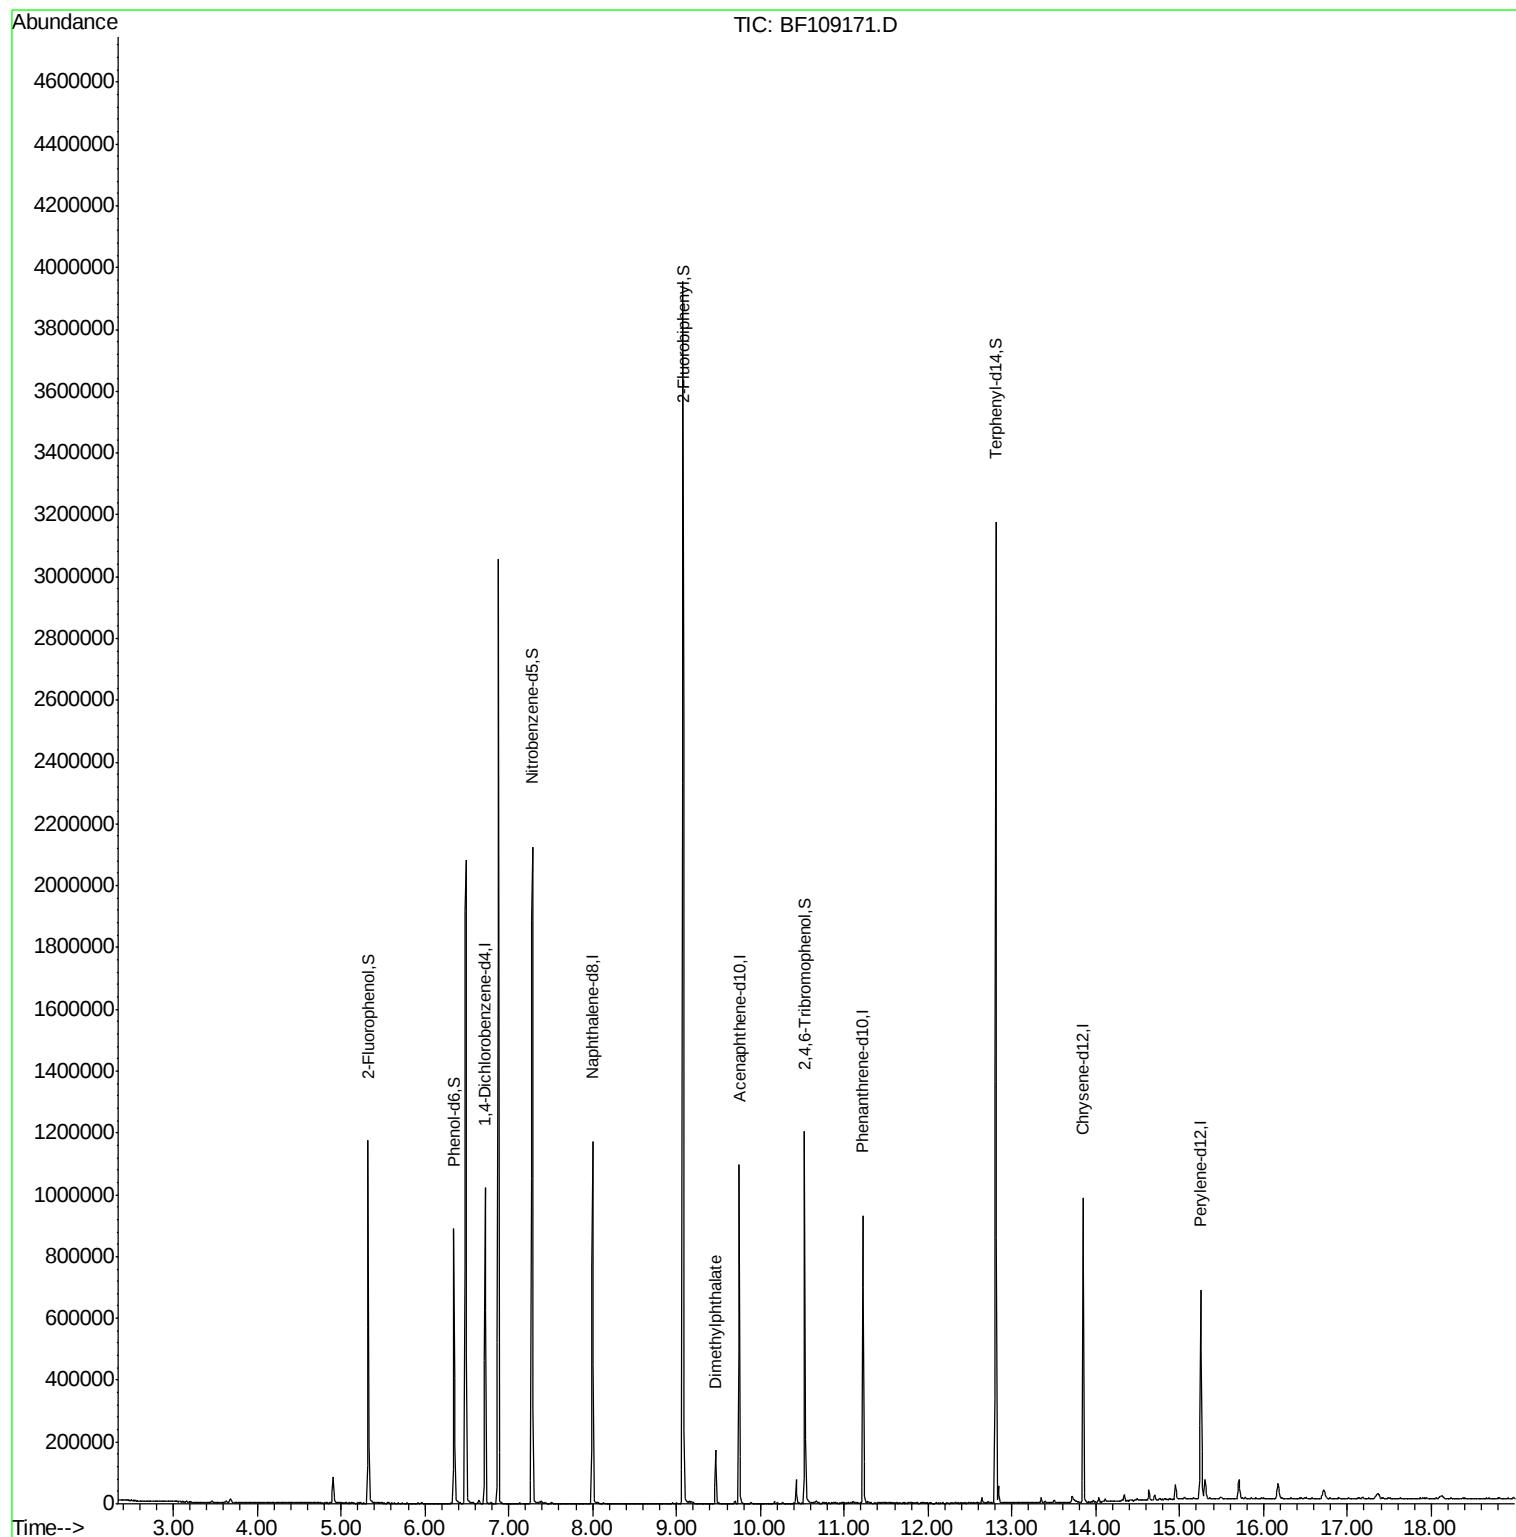




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.72 min Scan# 745
Delta R.T. -0.01 min
Lab File: BF109171.D
Acq: 20 Sep 2018 3:43

Instrument :
BNA_F
ClientSampleId :
091718-TIPC-E-D-M

Tot Ion:152 Resp: 136443
Ion Ratio Lower Upper
152 100
150 155.7 124.6 186.8
115 63.1 50.1 75.1

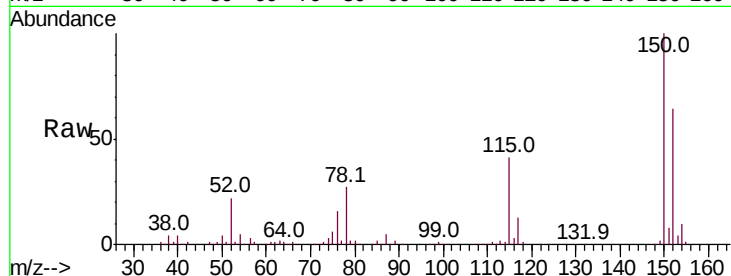


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

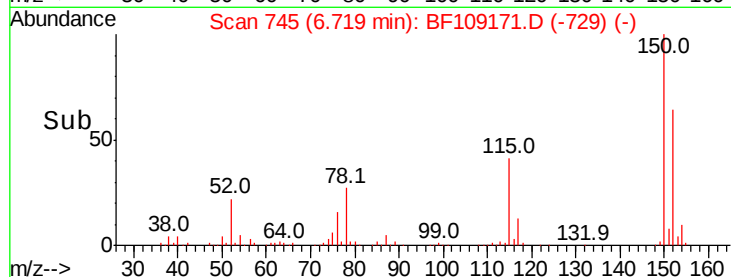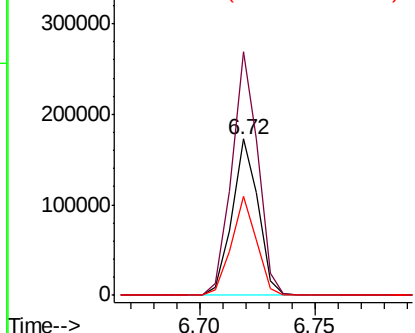



#5

2-Fluorophenol
Concen: 39.608 ng
RT: 5.32 min Scan# 508
Delta R.T. 0.00 min
Lab File: BF109171.D
Acq: 20 Sep 2018 3:43

Tgt Ion:112 Resp: 325386
Ion Ratio Lower Upper
112 100
64 59.3 47.9 71.9
63 31.2 23.7 35.5

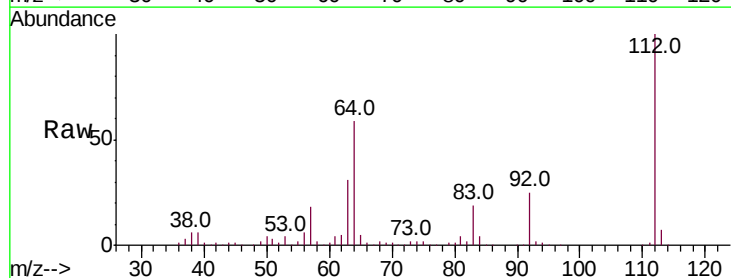

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

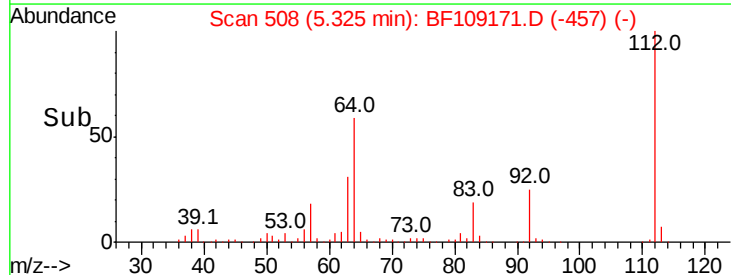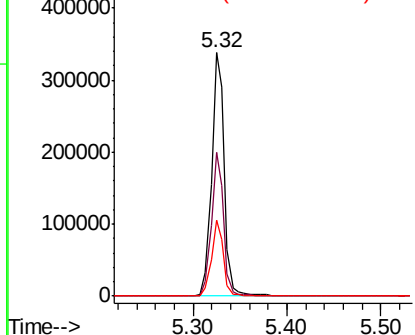



#7

Phenol-d6

Concen: 24.187 ng

RT: 6.35 min Scan# 682

Delta R.T. -0.01 min

Lab File: BF109171.D

Acq: 20 Sep 2018 3:43

Instrument :

BNA_F

ClientSampleId :

091718-TIPC-E-D-M


Tot Ion: 99 Resp: 256213

Ion Ratio Lower Upper




99 100

42 17.9 14.5 21.7

71 33.3 25.4 38.0

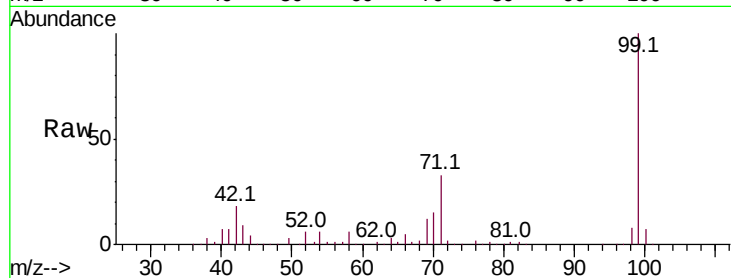

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

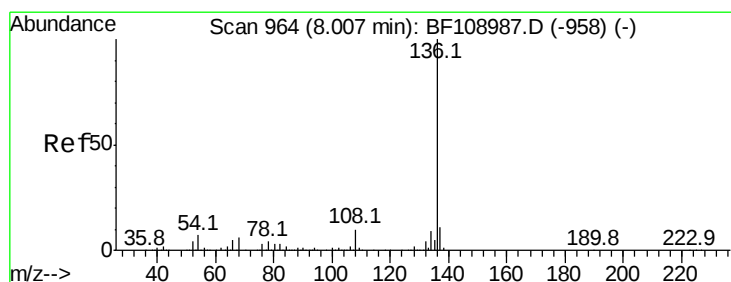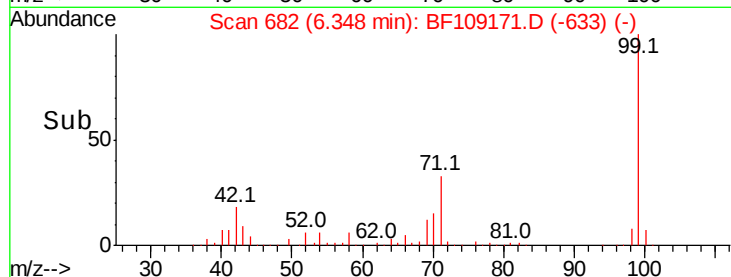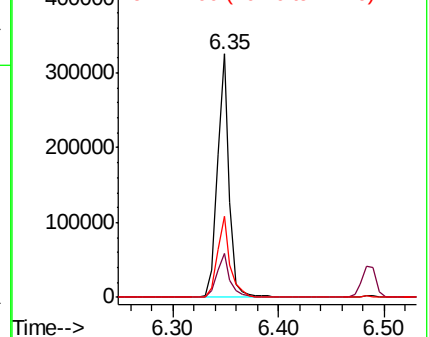

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.00 min Scan# 963

Delta R.T. -0.01 min

Lab File: BF109171.D

Acq: 20 Sep 2018 3:43

Tgt Ion: 136 Resp: 481379


Ion Ratio Lower Upper

136 100



137 11.0 8.9 13.3

54 6.7 6.6 9.8

68 5.5 5.0 7.4

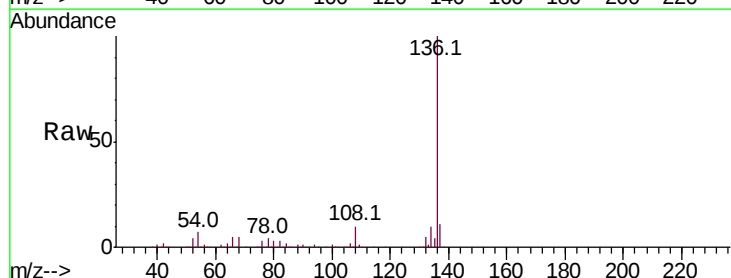

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

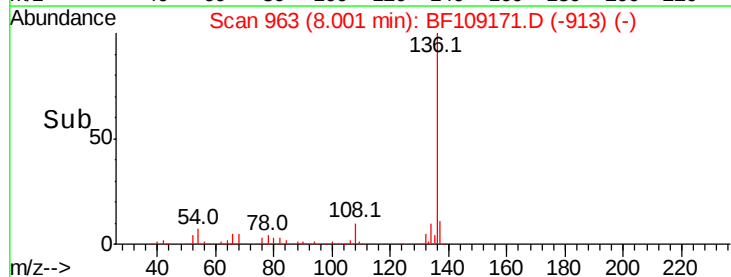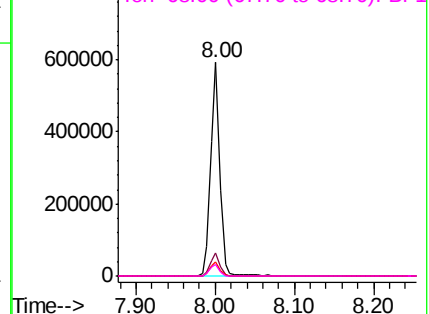







#23
Nitrobenzene-d5
Concen: 86.792 ng
RT: 7.28 min Scan# 841
Delta R.T. -0.01 min
Lab File: BF109171.D
Acq: 20 Sep 2018 3:43

Instrument :
BNA_F
ClientSampleId :
091718-TIPC-E-D-M

Tot Ion	82	Resp	744896
Ion	Ratio	Lower	Upper
82	100		
128	44.4	36.1	54.1
54	46.6	41.4	62.2

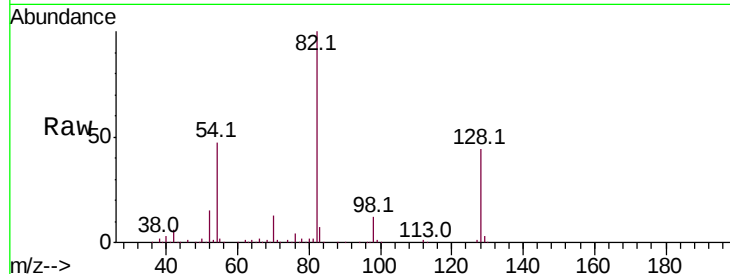


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

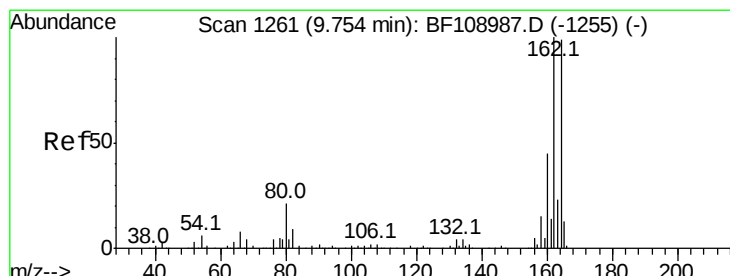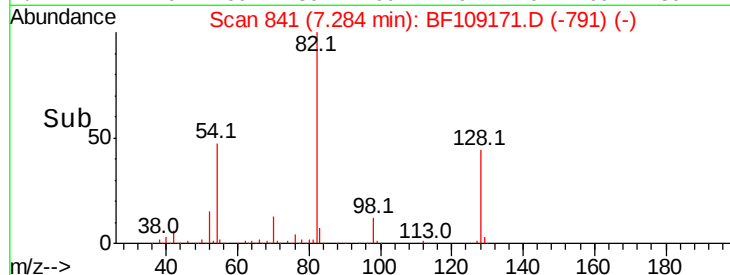
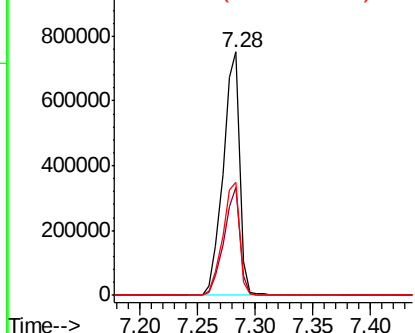


#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.75 min Scan# 1260
Delta R.T. -0.01 min
Lab File: BF109171.D
Acq: 20 Sep 2018 3:43

Tgt Ion	164	Resp	194036
Ion	Ratio	Lower	Upper
164	100		
162	102.7	86.1	129.1
160	46.1	38.3	57.5

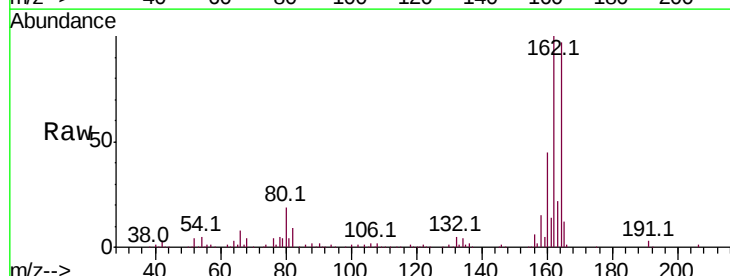

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

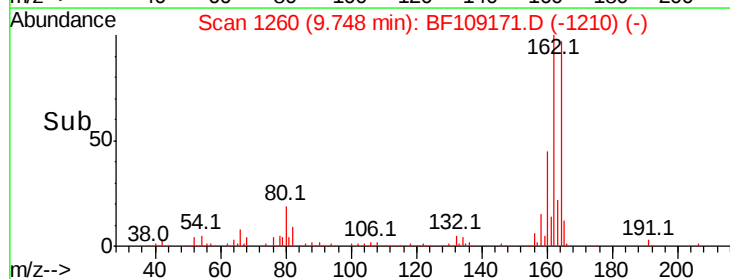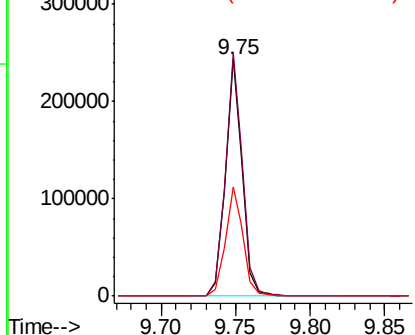






#41
 2,4,6-Tribromophenol
 Concen: 68.486 ng
 RT: 10.53 min Scan# 1393
 Delta R.T. -0.01 min
 Lab File: BF109171.D
 Acq: 20 Sep 2018 3:43

Instrument :
 BNA_F
 ClientSampleId :
 091718-TIPC-E-D-M

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.2	77.0	115.6
141	31.8	29.9	44.9

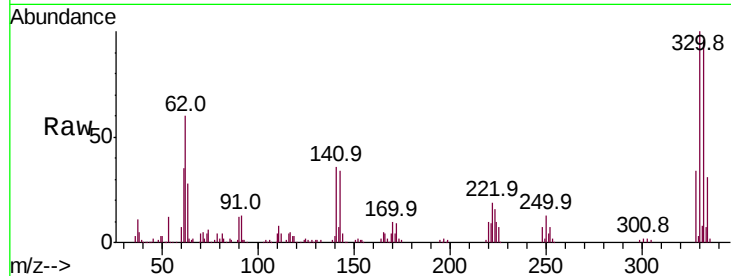


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

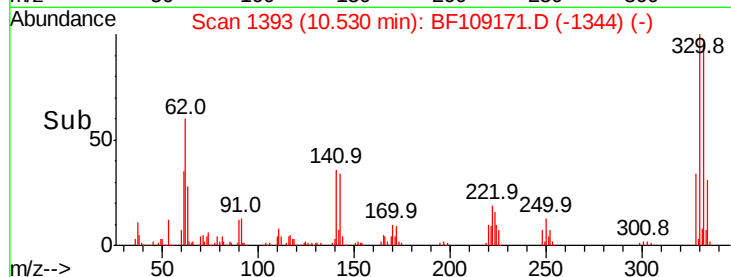
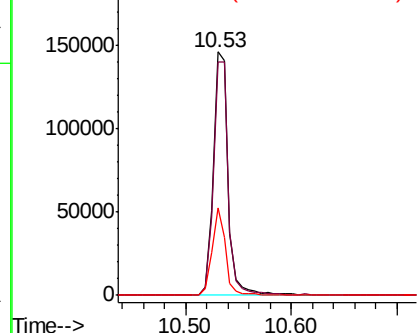



#44
 2-Fluorobiphenyl
 Concen: 99.221 ng
 RT: 9.08 min Scan# 1146
 Delta R.T. -0.01 min
 Lab File: BF109171.D
 Acq: 20 Sep 2018 3:43

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.6	29.7	44.5
170	24.4	19.6	29.4

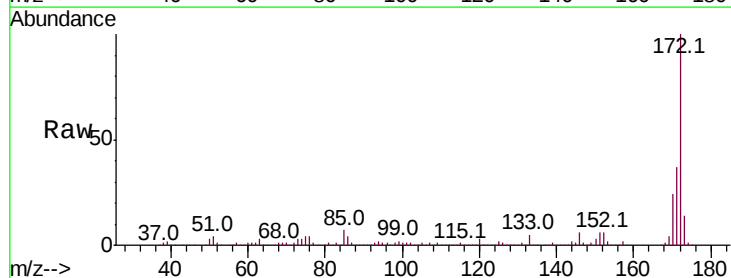

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

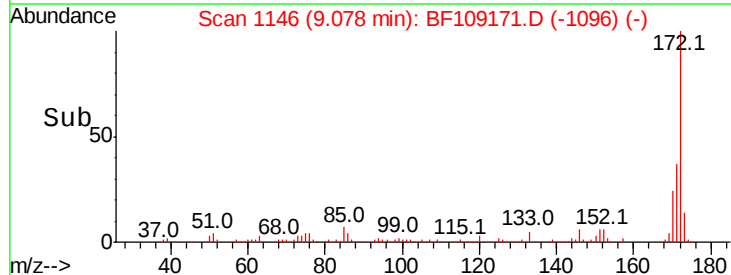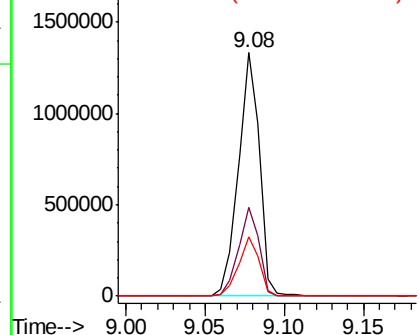

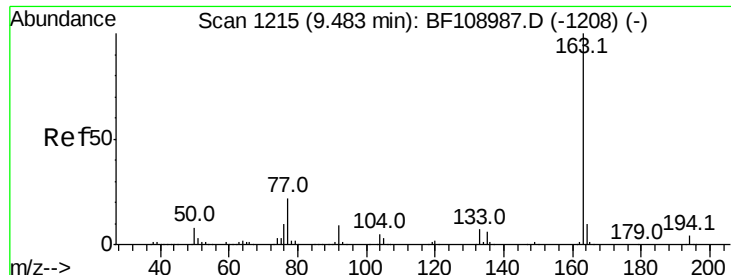

#49

Dimethylphthalate

Concen: 4.978 ng

RT: 9.47 min Scan# 1212

Delta R.T. -0.02 min

Lab File: BF109171.D

Acq: 20 Sep 2018 3:43

Instrument :

BNA_F

ClientSampleId :

091718-TIPC-E-D-M


Tot Ion:163 Resp: 69040

Ion Ratio Lower Upper




163 100

194 3.4 2.7 4.1

164 10.5 8.2 12.2

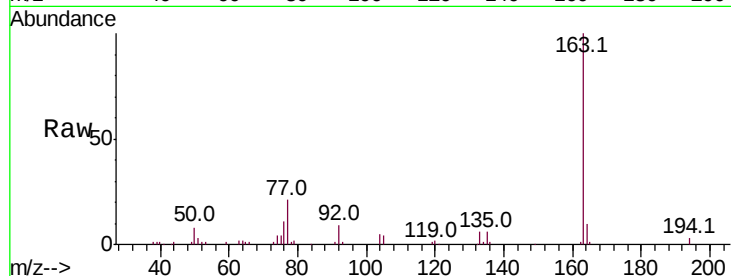

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

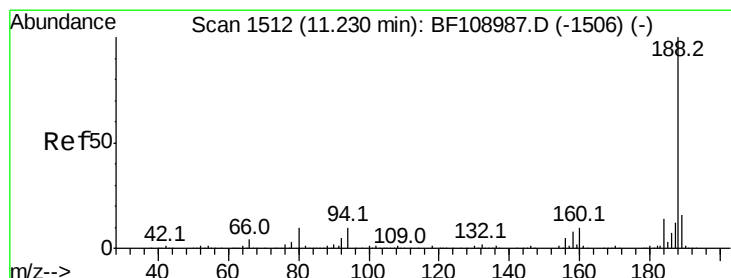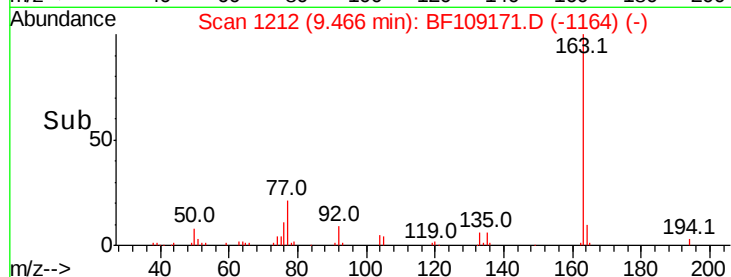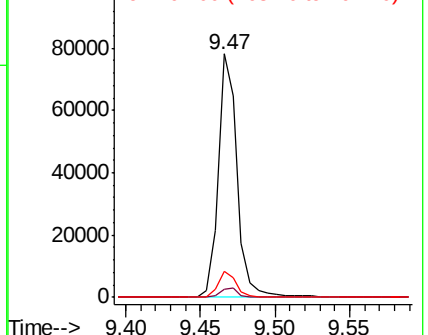

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.22 min Scan# 1511

Delta R.T. -0.01 min

Lab File: BF109171.D

Acq: 20 Sep 2018 3:43


Tgt Ion:188 Resp: 328568

Ion Ratio Lower Upper



188 100

94 10.2 8.5 12.7

80 10.8 9.2 13.8

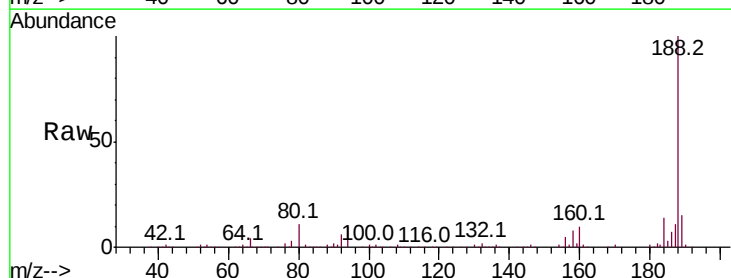

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

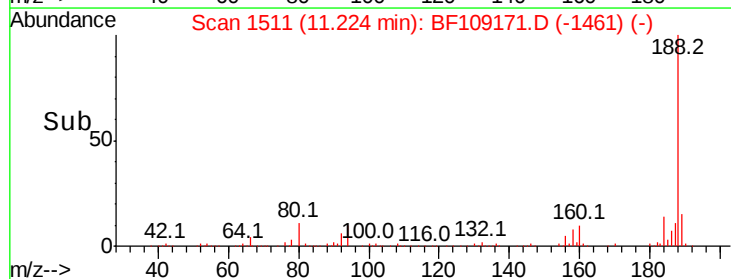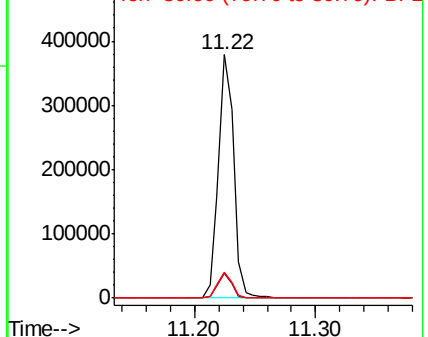



#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.85 min Scan# 1957

Delta R.T. -0.01 min

Lab File: BF109171.D

Acq: 20 Sep 2018 3:43

Instrument :

BNA_F

ClientSampleId :

091718-TIPC-E-D-M


Tot Ion:240 Resp: 337661

Ion Ratio Lower Upper




240 100

120 12.2 9.5 14.3

236 25.7 20.7 31.1

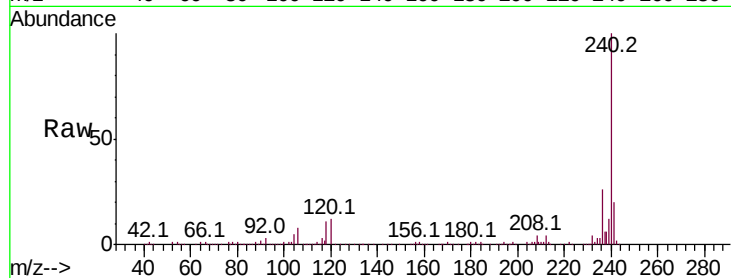

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

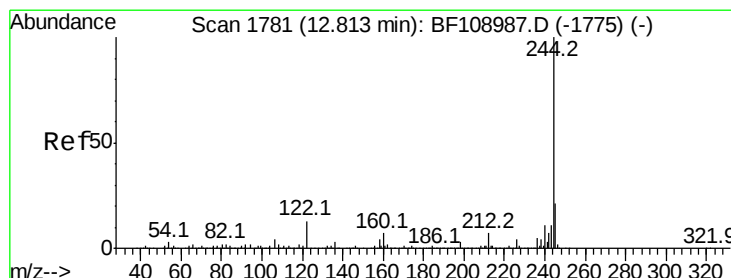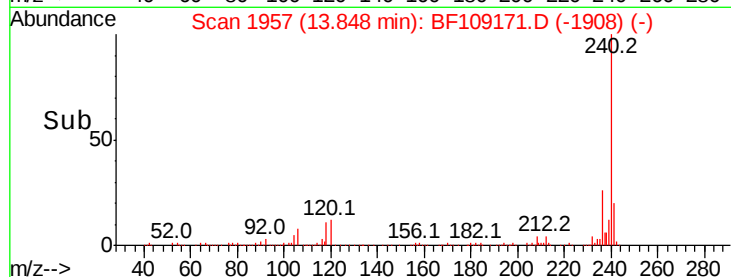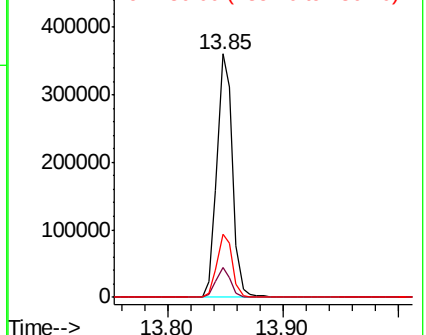

#78

Terphenyl-d14

Concen: 78.467 ng

RT: 12.81 min Scan# 1781

Delta R.T. -0.00 min

Lab File: BF109171.D

Acq: 20 Sep 2018 3:43


Tgt Ion:244 Resp: 1117813

Ion Ratio Lower Upper



244 100


212 6.9 5.4 8.0

122 10.8 11.0 16.4#

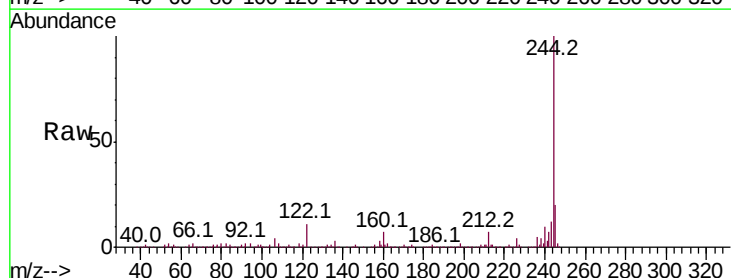

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

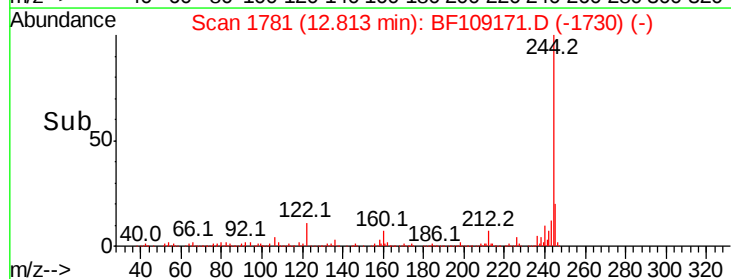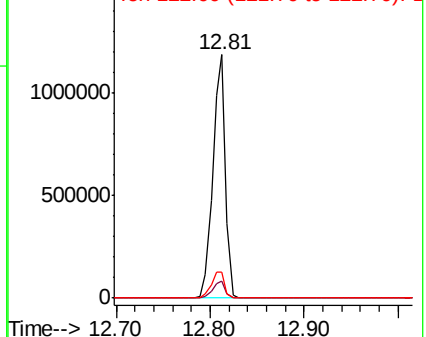

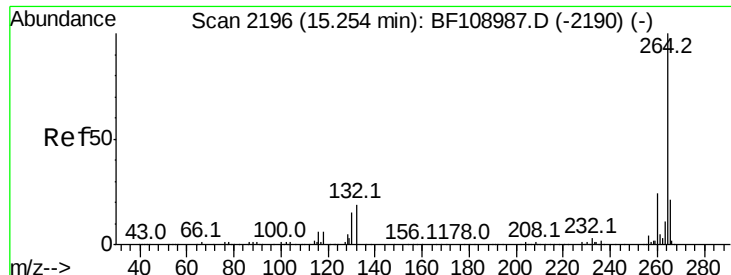

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.25 min Scan# 2196
Delta R.T. -0.00 min
Lab File: BF109171.D
Acq: 20 Sep 2018 3:43

Instrument :
BNA_F
ClientSampleId :
091718-TIPC-E-D-M

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.2	28.8
265	21.8	17.5	26.3

