


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091918\
 Data File : BF109139.D
 Acq On : 19 Sep 2018 13:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 14 13:26:52 2018

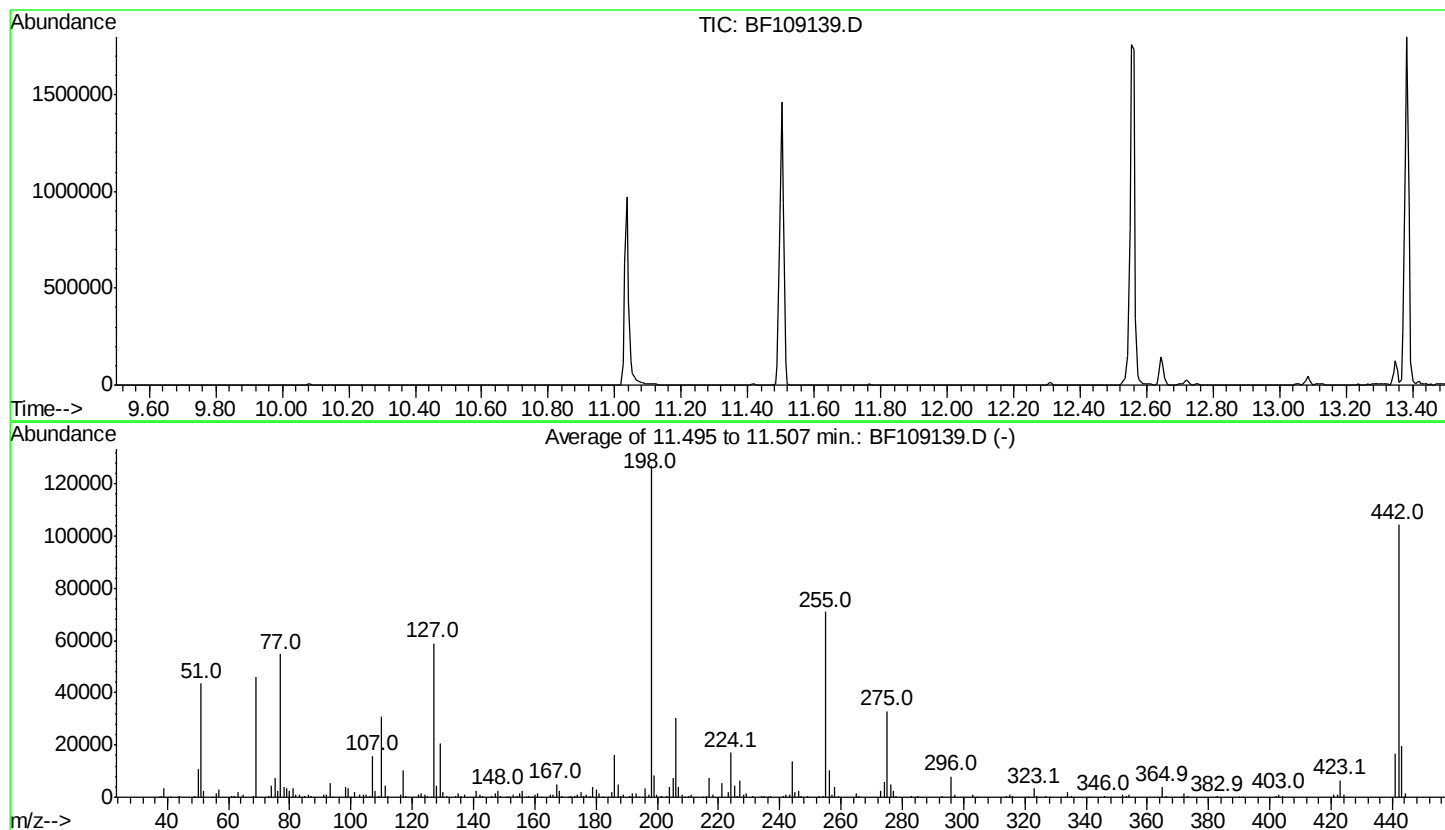

AutoFind: Scans 1557, 1558, 1559; Background Corrected with Scan 1552

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	43562	PASS
68	69	0.00	2	1.6	717	PASS
69	198	0.00	100	36.2	46016	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.5	59042	PASS
197	198	0.00	2	0.8	1014	PASS
198	198	100	100	100.0	126997	PASS
199	198	5	9	6.7	8465	PASS
275	198	10	60	25.9	32952	PASS
365	198	1	100	3.3	4181	PASS
441	198	0.01	100	13.2	16739	PASS
442	198	50	100	82.1	104213	PASS
443	442	15	24	18.8	19558	PASS