


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091918\
 Data File : BF109166.D
 Acq On : 20 Sep 2018 1:27
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 14 13:26:52 2018

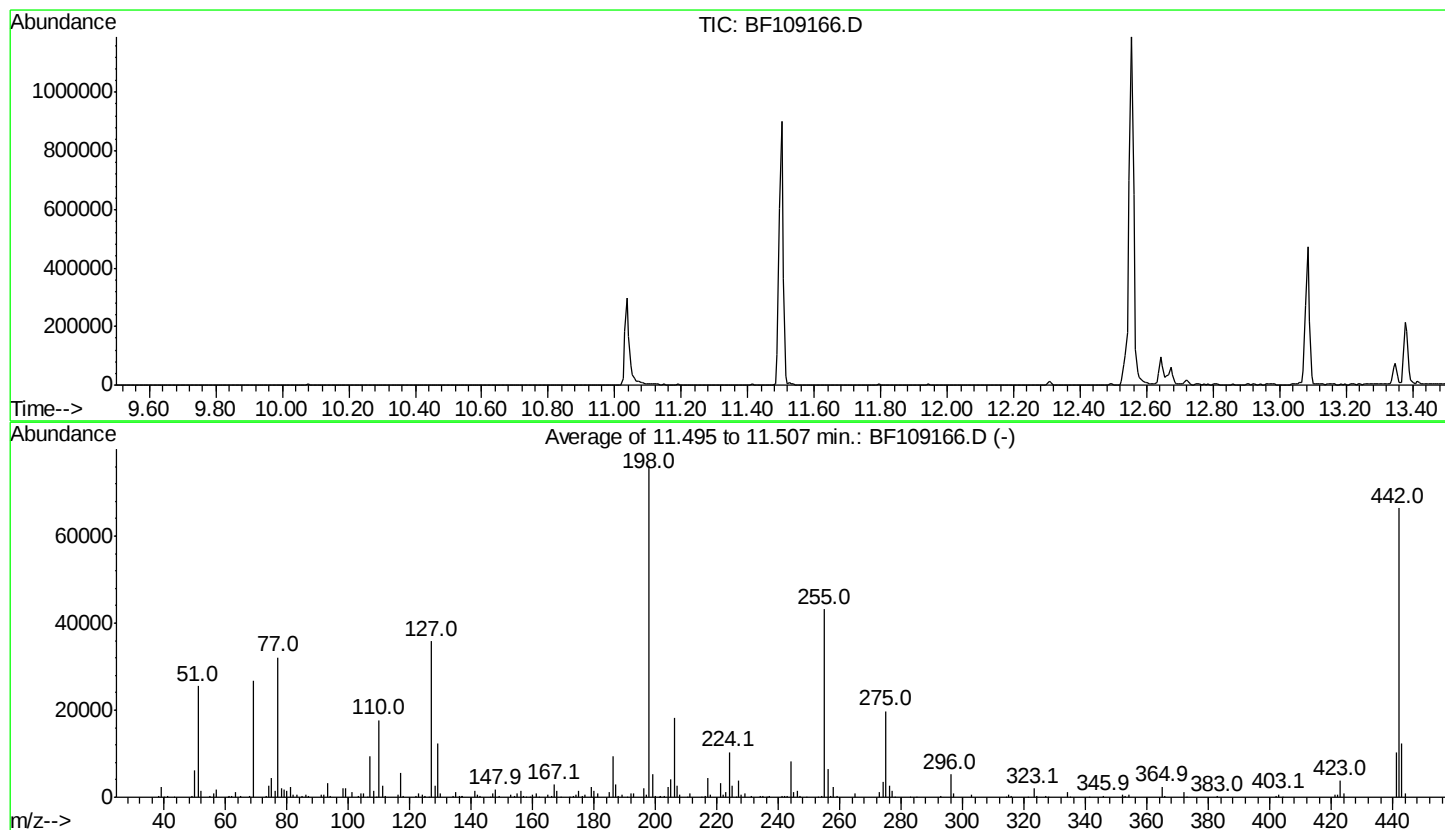

AutoFind: Scans 1557, 1558, 1559; Background Corrected with Scan 1552

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	25552	PASS
68	69	0.00	2	1.4	363	PASS
69	198	0.00	100	35.2	26821	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.1	35866	PASS
197	198	0.00	2	0.9	659	PASS
198	198	100	100	100.0	76189	PASS
199	198	5	9	7.1	5447	PASS
275	198	10	60	26.0	19812	PASS
365	198	1	100	3.1	2399	PASS
441	198	0.01	100	13.5	10250	PASS
442	198	50	100	87.1	66397	PASS
443	442	15	24	18.7	12448	PASS