
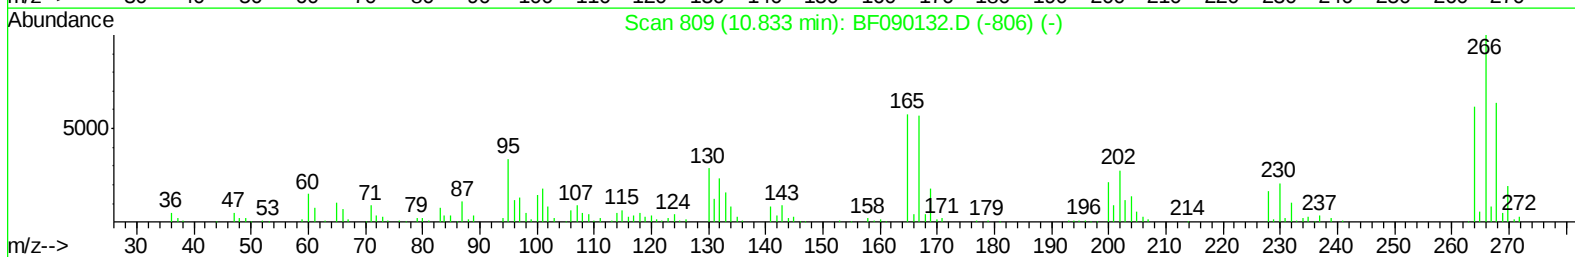
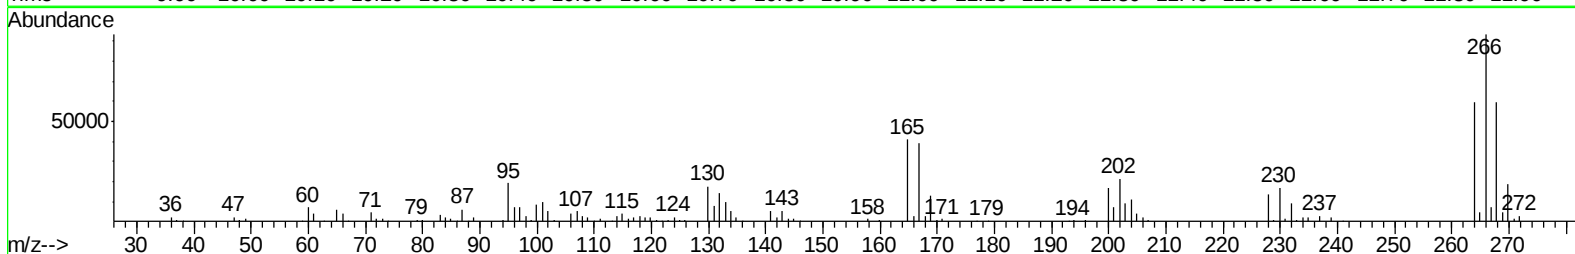


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092016\
Data File : BF090137.D
Acq On : 20 Sep 2016 16:41
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 04:22:53 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 17:58:29 2016
Response via : Initial Calibration

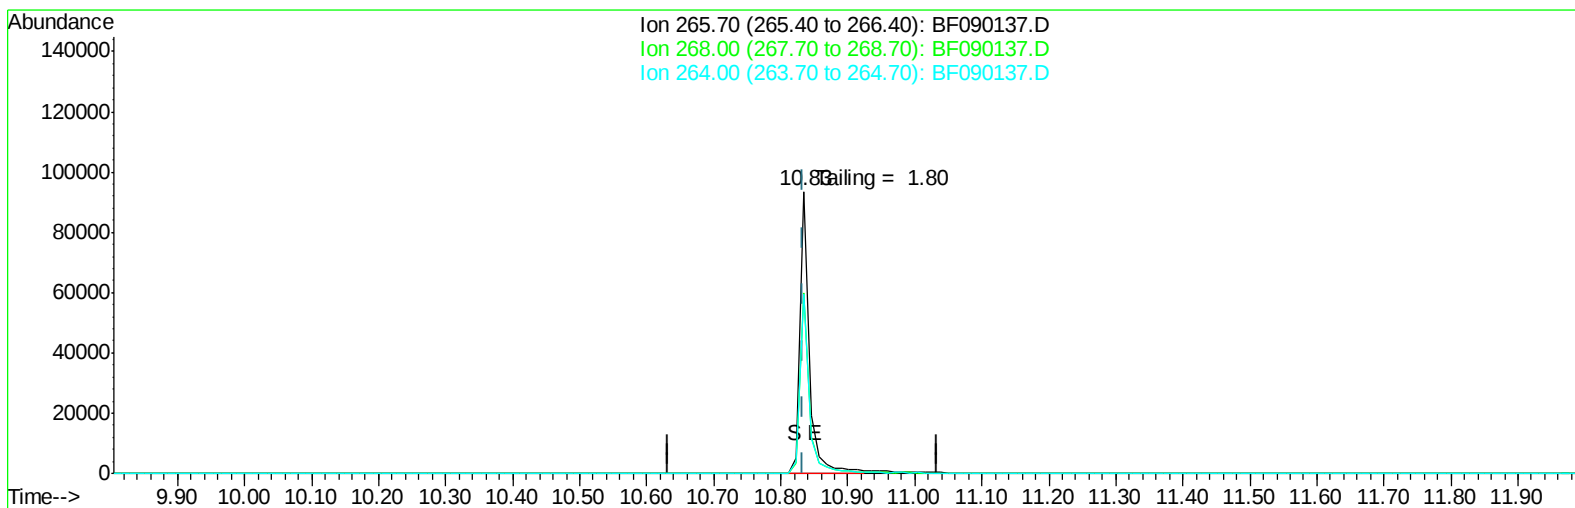

TIC: BF090137.D

(69) Pentachlorophenol (C)




10.833min (-0.000) 0.00ng

response 93608

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	63.90
264.00	62.90	63.64
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092016\
Data File : BF090137.D
Acq On : 20 Sep 2016 16:41
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 04:22:53 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 17:58:29 2016
Response via : Initial Calibration

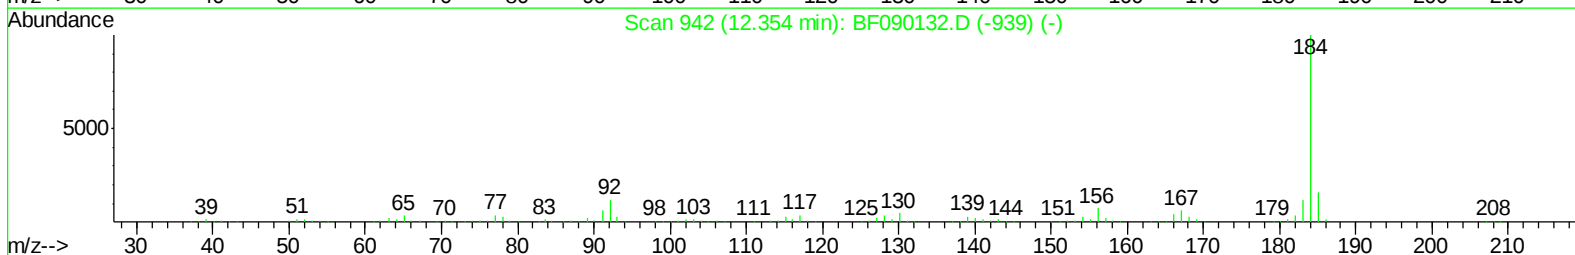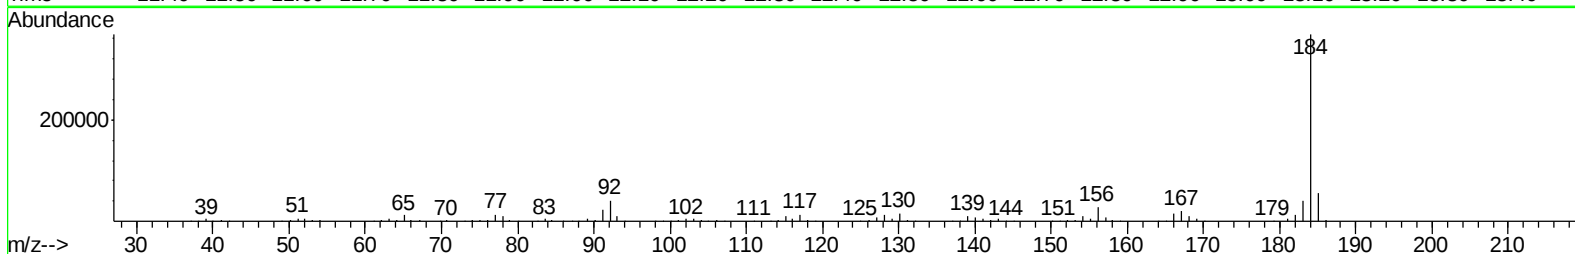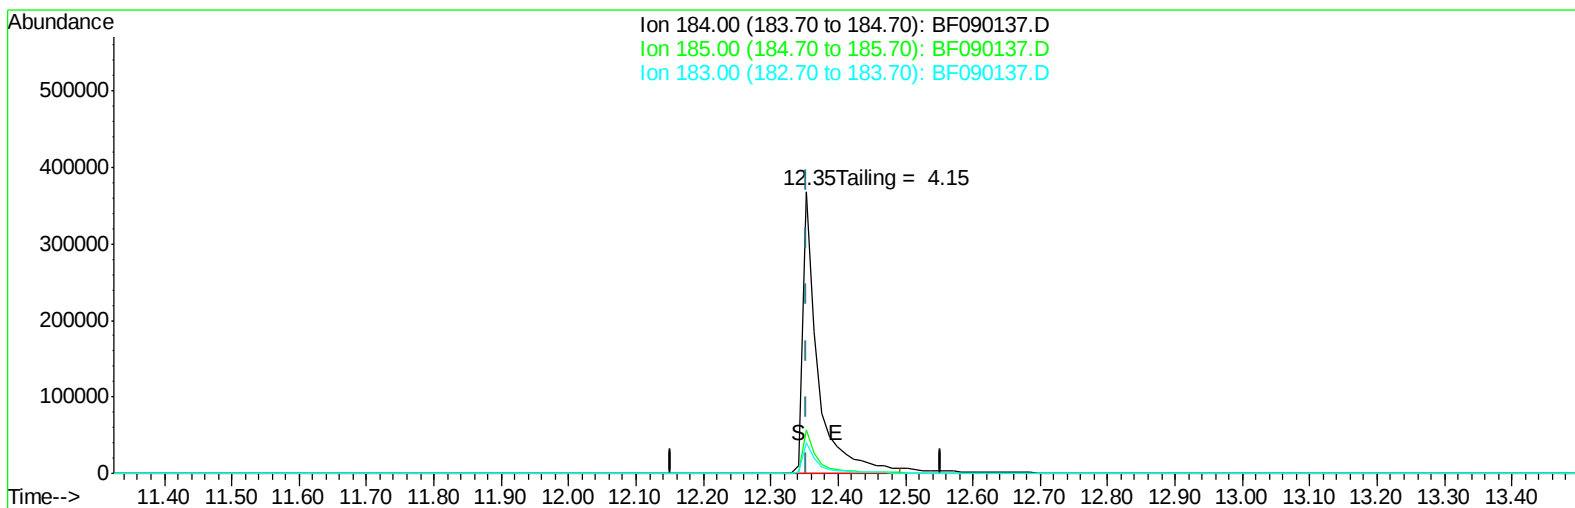

TIC: BF090137.D

(76) Benzidine

12.354min (+0.001) 0.00ng

response 576507

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	15.43
183.00	11.50	11.00
0.00	0.00	0.00