


Data Path : Z:\HPCHEM1\BNA F\DATA\BF092016\
 Data File : BF090128.D
 Acq On : 20 Sep 2016 10:00
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 20 17:58:29 2016

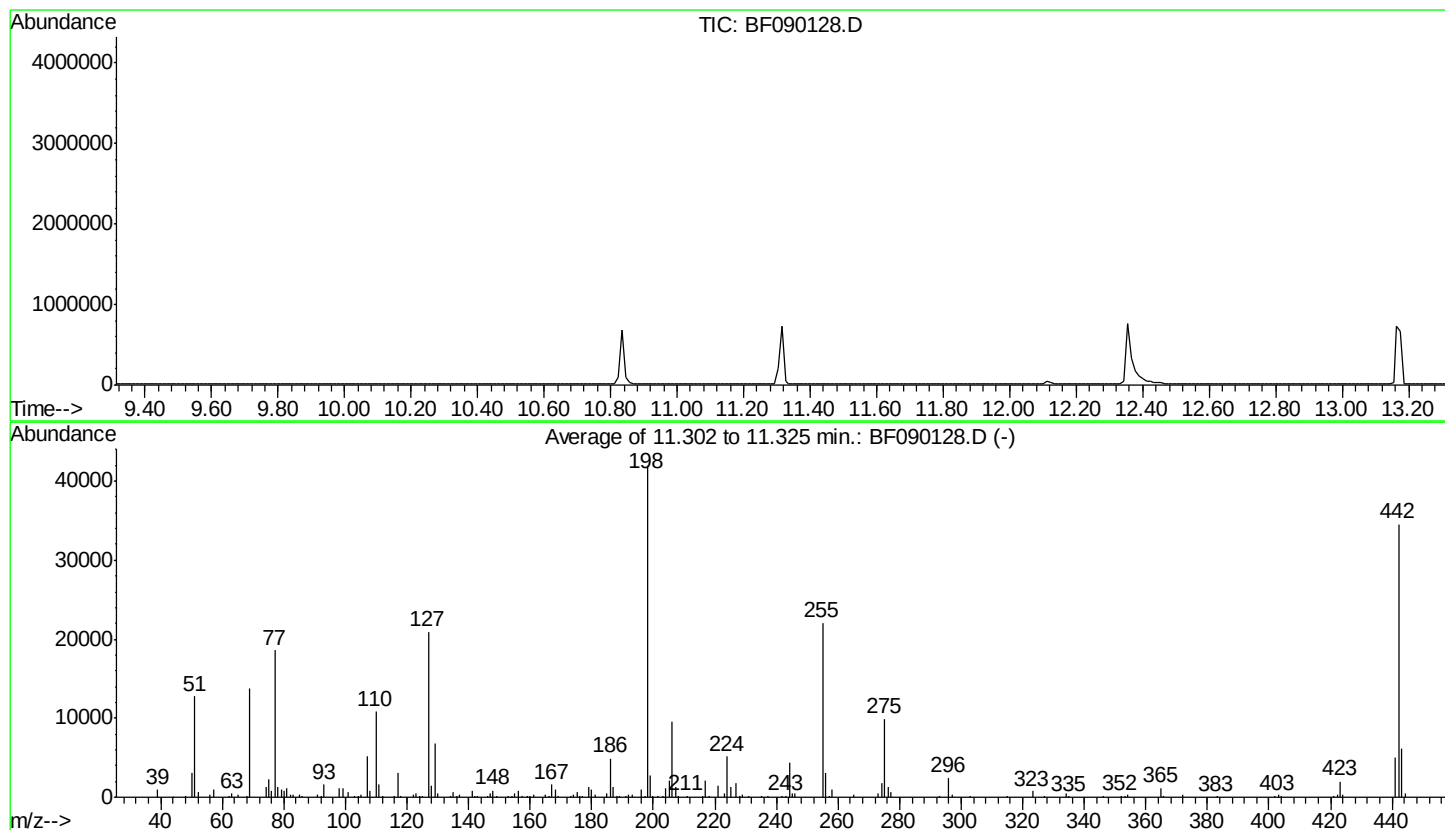

AutoFind: Scans 850, 851, 852; Background Corrected with Scan 847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	12778	PASS
68	69	0.00	2	1.7	237	PASS
69	198	0.00	100	33.0	13832	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.9	20921	PASS
197	198	0.00	2	0.6	244	PASS
198	198	100	100	100.0	41957	PASS
199	198	5	9	6.5	2709	PASS
275	198	10	60	23.7	9953	PASS
365	198	1	100	2.8	1163	PASS
441	442	0.01	24	14.6	5032	PASS
442	198	50	100	82.4	34583	PASS
443	442	15	24	18.0	6214	PASS