


Data Path : Z:\HPCHEM1\BNA F\Data\BF092016\
 Data File : BF090137.D
 Acq On : 20 Sep 2016 16:41
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 20 17:58:29 2016

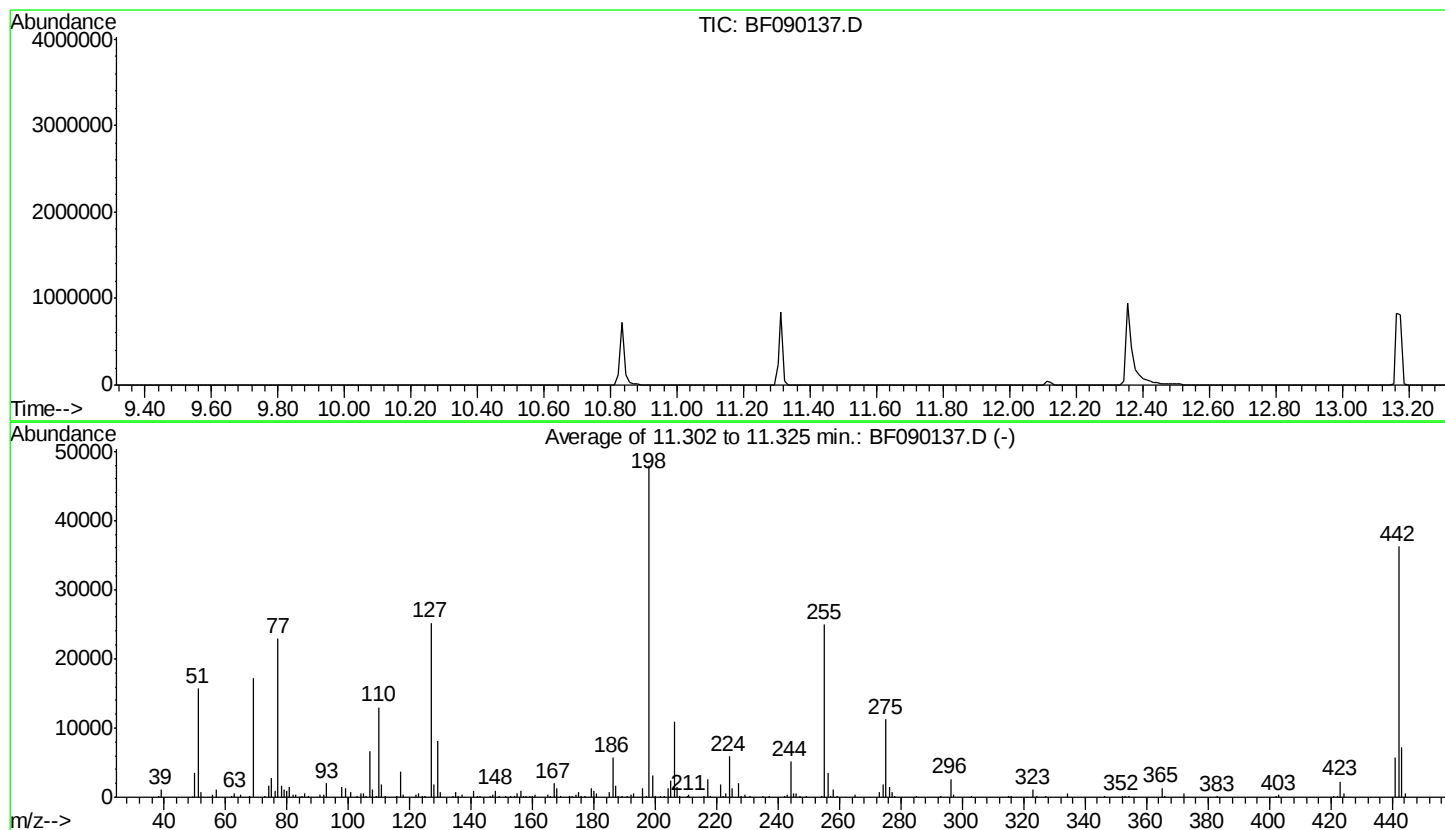

AutoFind: Scans 850, 851, 852; Background Corrected with Scan 846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	15645	PASS
68	69	0.00	2	1.6	273	PASS
69	198	0.00	100	36.1	17278	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.5	25175	PASS
197	198	0.00	2	0.5	240	PASS
198	198	100	100	100.0	47920	PASS
199	198	5	9	6.7	3205	PASS
275	198	10	60	23.4	11202	PASS
365	198	1	100	2.8	1336	PASS
441	442	0.01	24	15.9	5766	PASS
442	198	50	100	75.6	36232	PASS
443	442	15	24	19.7	7139	PASS