


Data Path : Z:\HPCHEM1\BNA_F\Data\BF092017\
 Data File : BF098653.D
 Acq On : 20 Sep 2017 10:53
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 18 13:37:24 2017

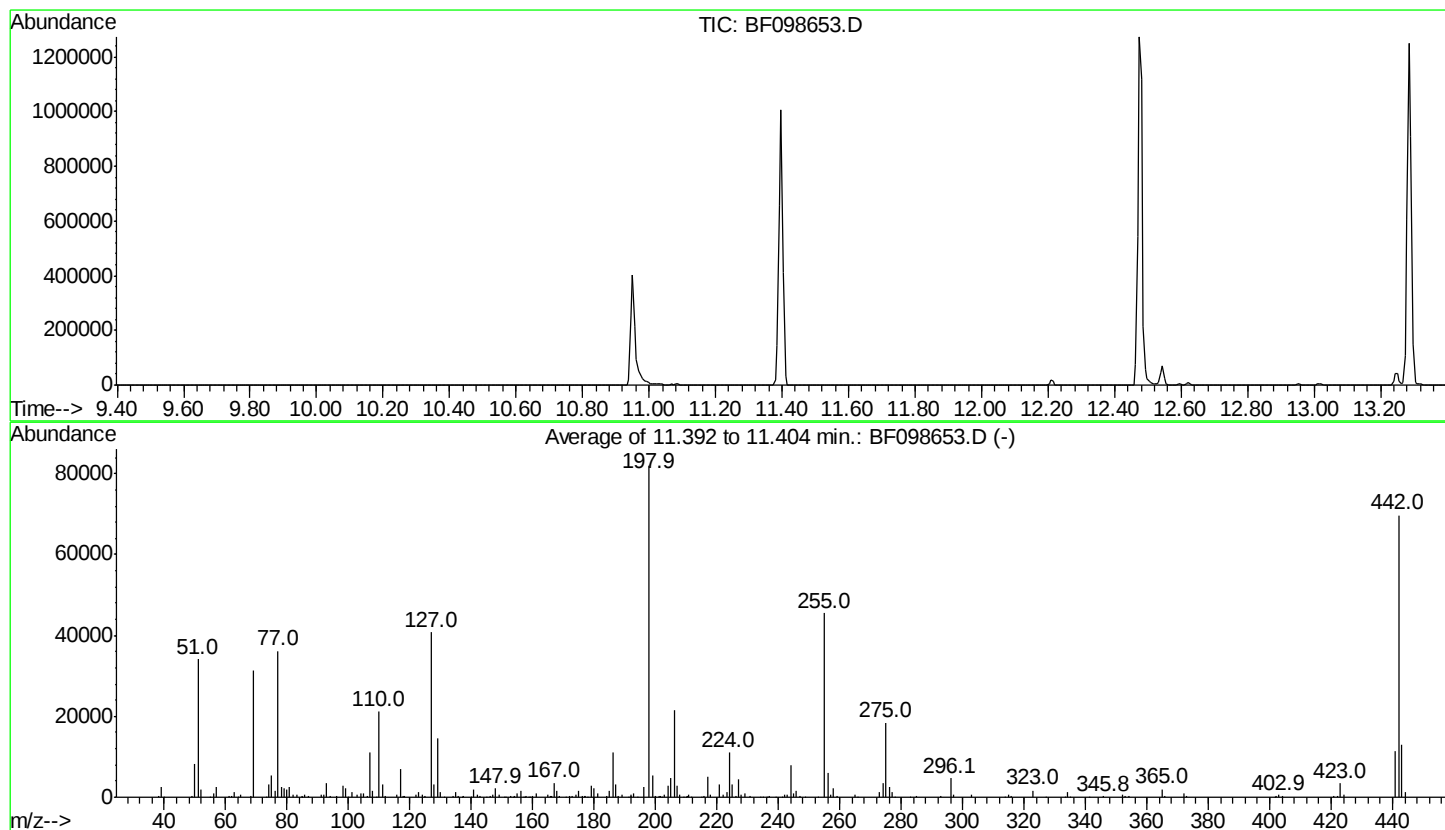

AutoFind: Scans 1582, 1583, 1584; Background Corrected with Scan 1576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	34175	PASS
68	69	0.00	2	1.5	473	PASS
69	198	0.00	100	38.4	31478	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.6	40704	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81997	PASS
199	198	5	9	6.6	5383	PASS
275	198	10	60	22.5	18487	PASS
365	198	1	100	2.4	1962	PASS
441	442	0.01	24	16.3	11377	PASS
442	198	50	100	85.0	69698	PASS
443	442	15	24	18.8	13133	PASS