


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092024\
Data File : BF139492.D
Acq On : 20 Sep 2024 09:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 14 02:58:23 2024

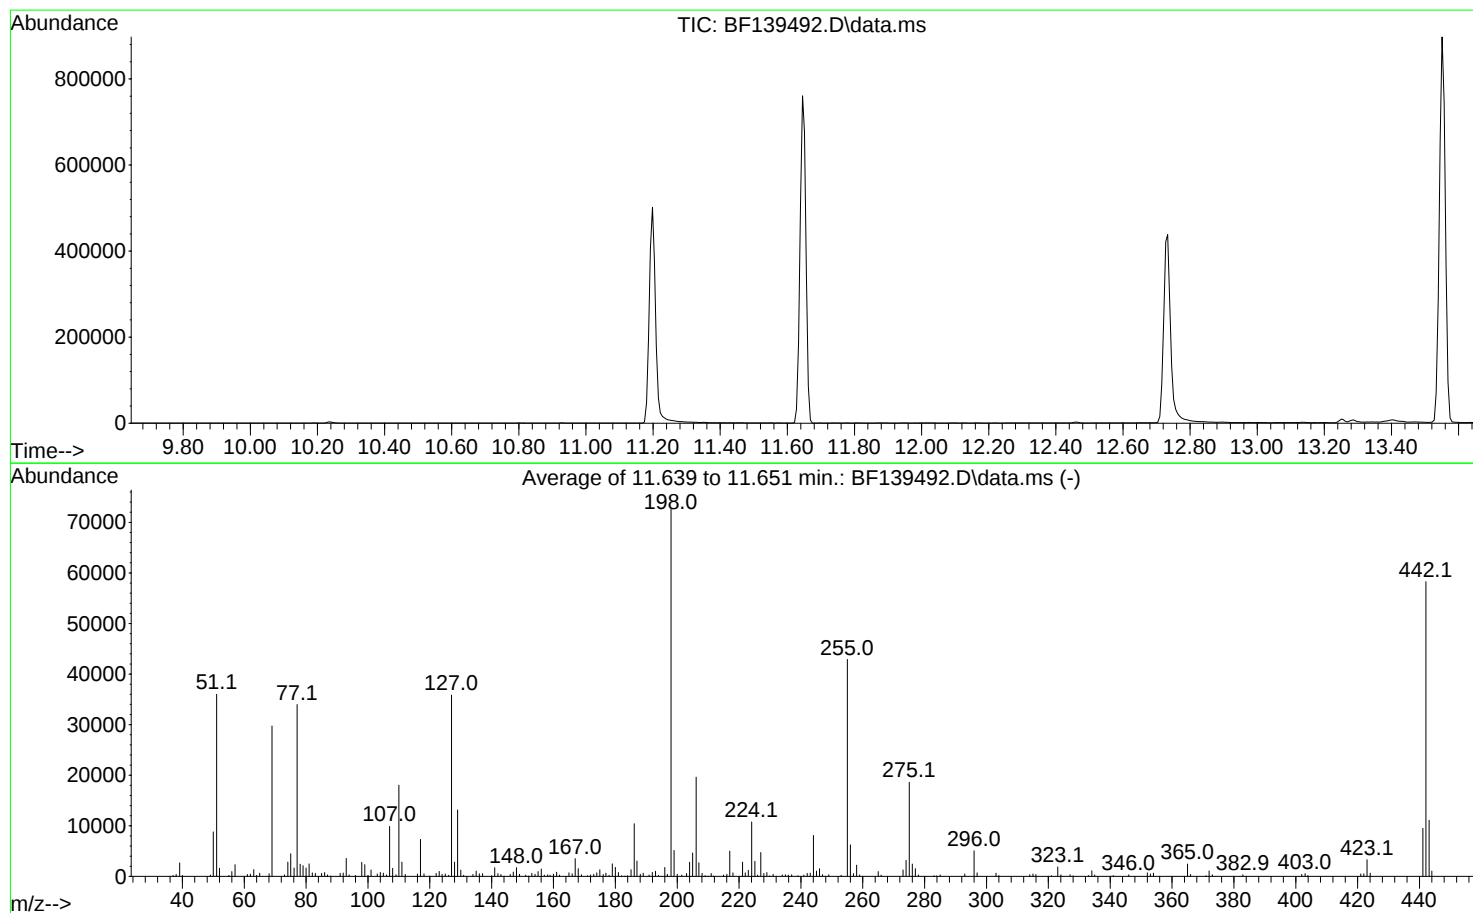

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.5	36000	PASS
68	69	0.00	2	1.7	497	PASS
69	198	0.00	100	40.9	29744	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.3	35861	PASS
197	198	0.00	2	0.6	407	PASS
198	198	100	100	100.0	72741	PASS
199	198	5	9	7.1	5134	PASS
275	198	10	60	25.6	18621	PASS
365	198	1	100	3.4	2450	PASS
441	198	0.01	100	13.0	9490	PASS
442	442	50	100	100.0	58267	PASS
443	442	15	24	19.1	11107	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/20/2024	BNA_F	<u>BF139492.D</u>
Compound Name	Response	Retention Time
DDT	217300	13.551
DDD	4913	13.251
DDE	121	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5034	222334	2.26

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092024\
Data File : BF139492.D
Acq On : 20 Sep 2024 09:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 20 11:15:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

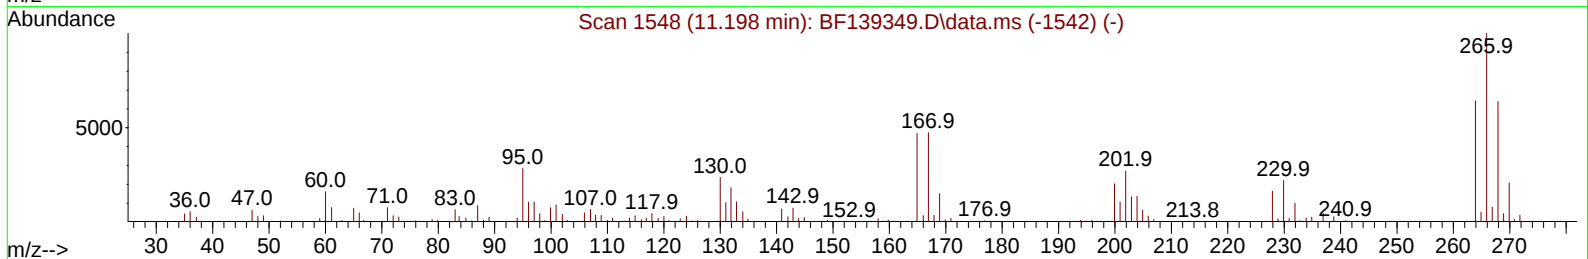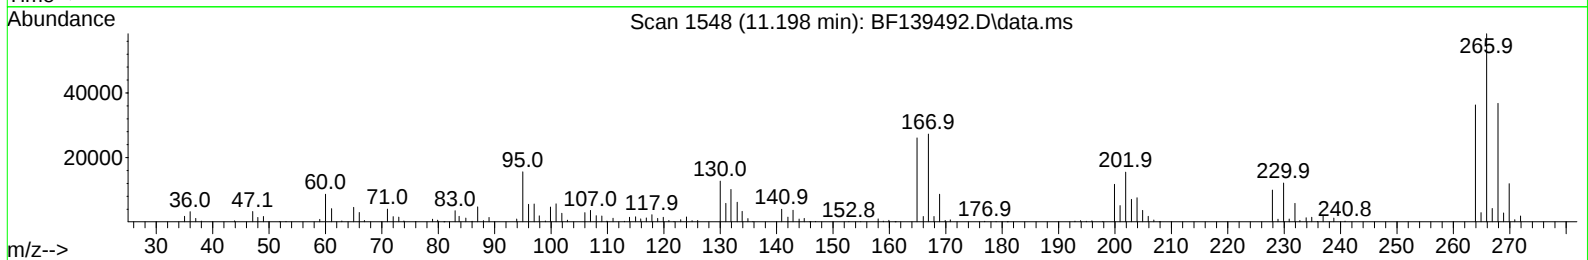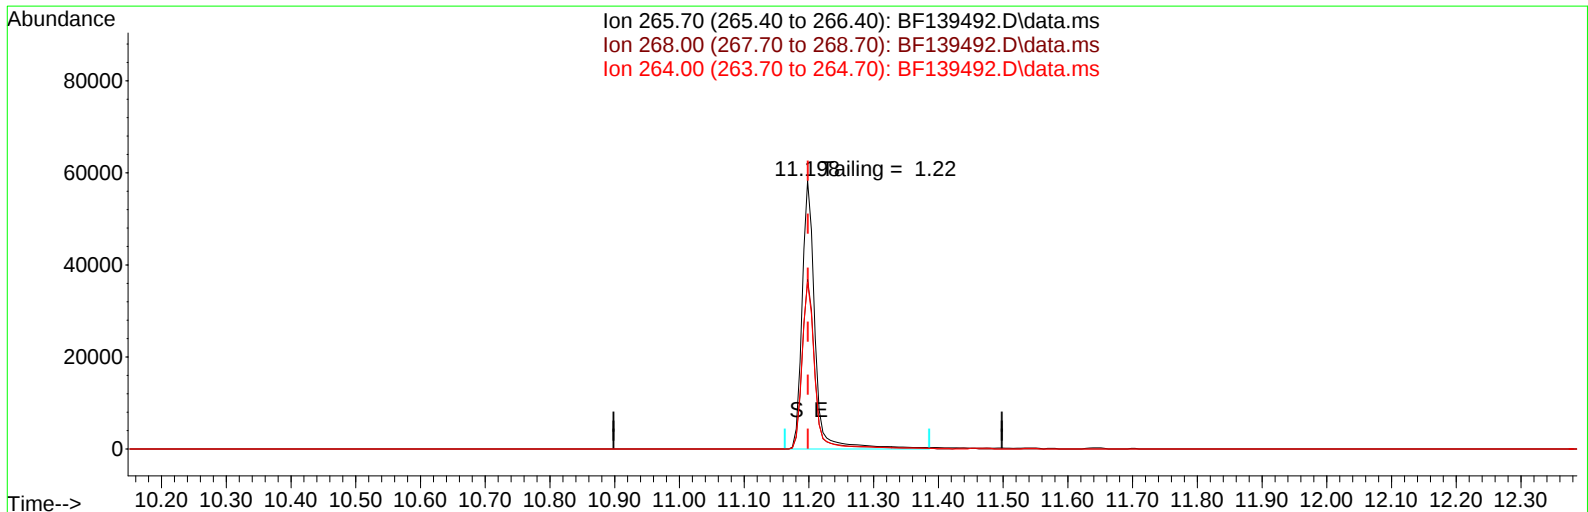

TIC: BF139492.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 23398.77 ng




response 81483

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.11
264.00	64.20	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092024\
Data File : BF139492.D
Acq On : 20 Sep 2024 09:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 20 11:15:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

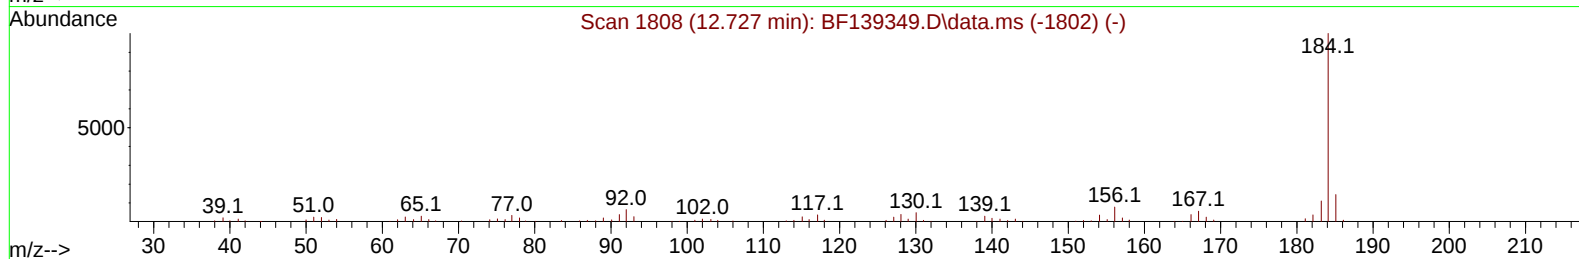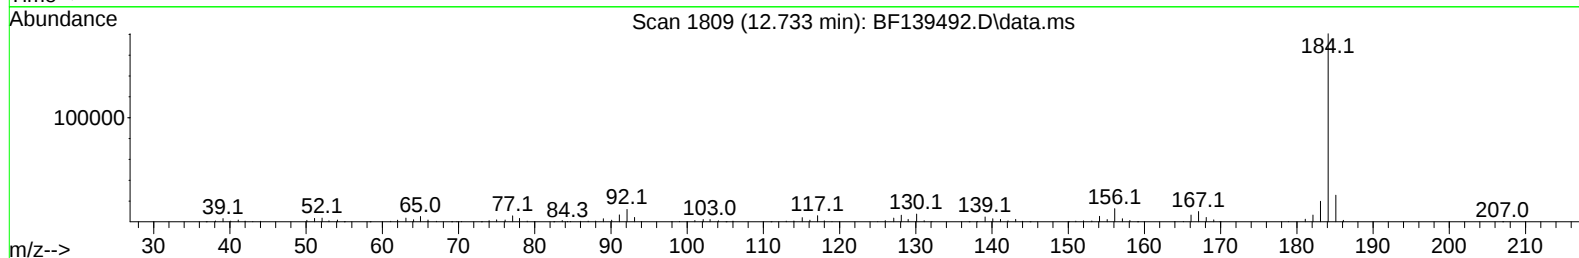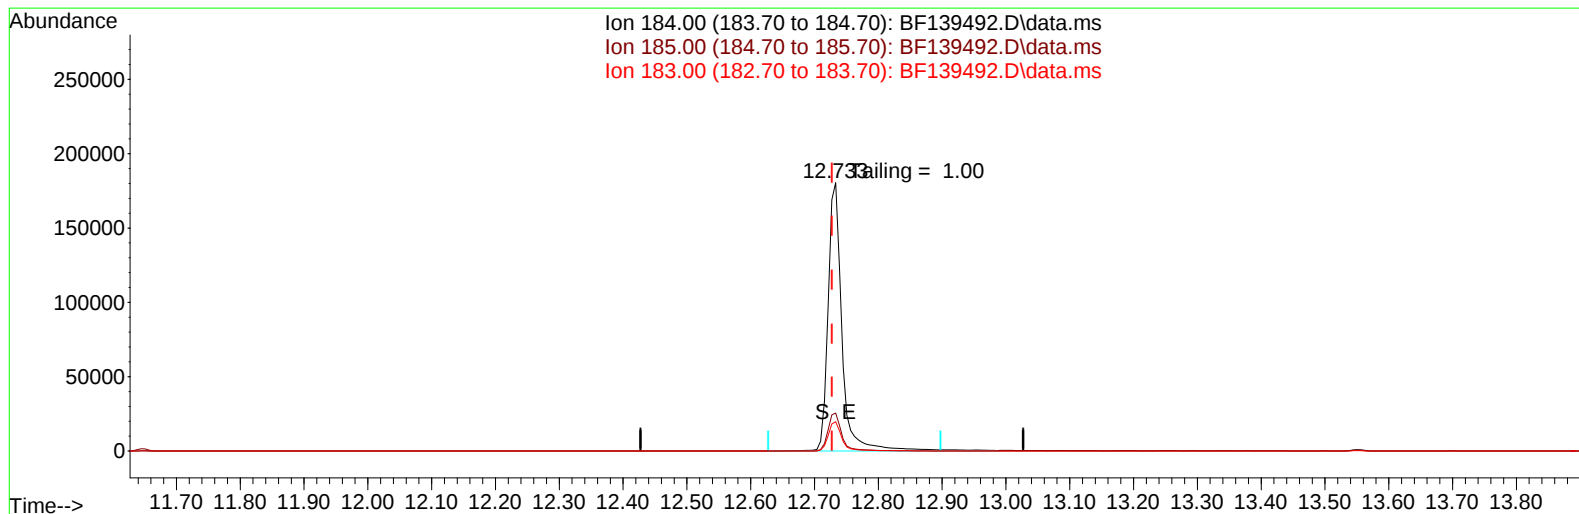

TIC: BF139492.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 0.00 ng

response 273652

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.17
183.00	11.10	10.95
0.00	0.00	0.00