


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092115\
 Data File : BF081709.D
 Acq On : 21 Sep 2015 11:43
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 22 17:42:58 2015

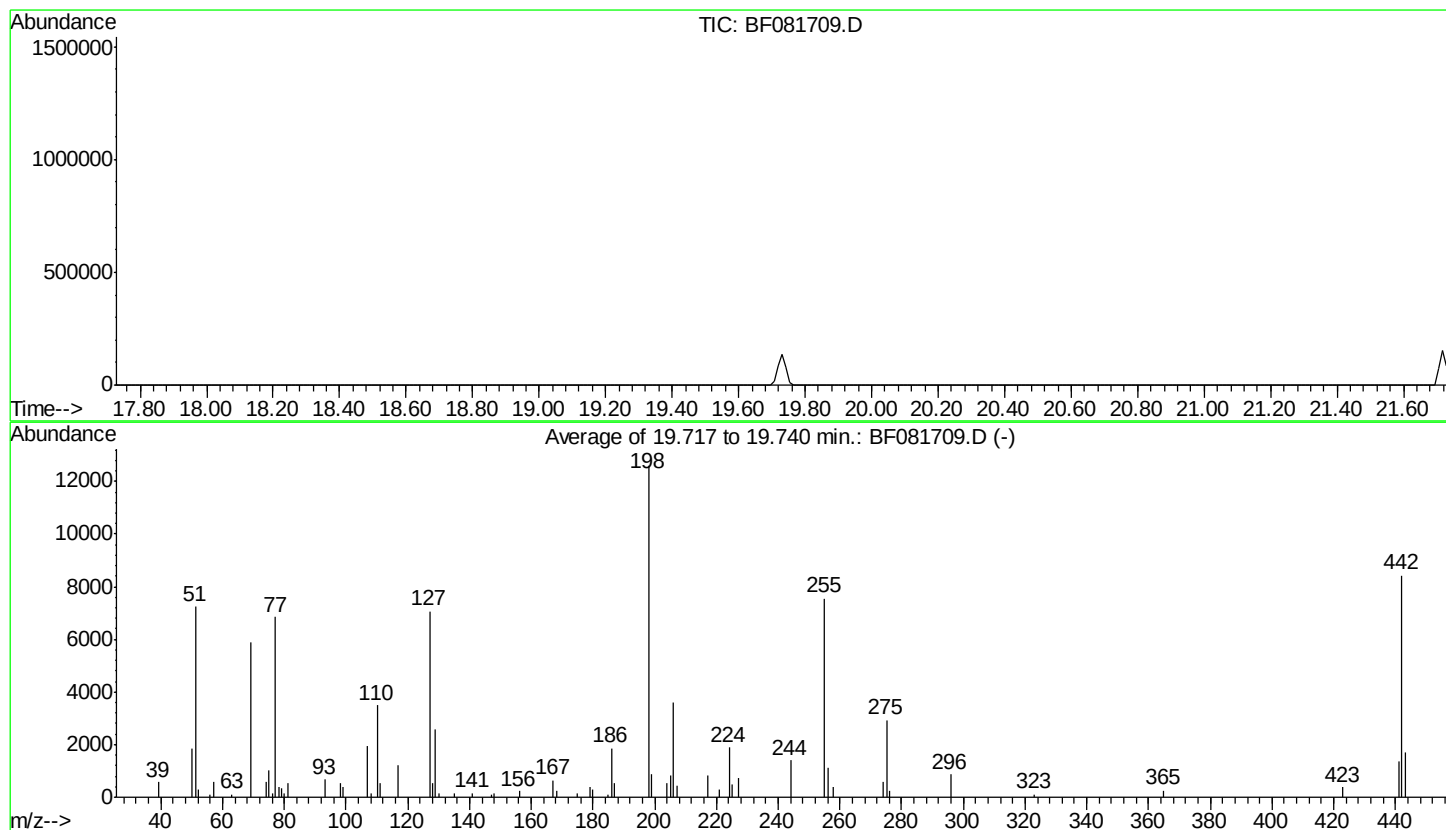

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.5	7243	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.7	5891	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.0	7057	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12602	PASS
199	198	5	9	6.8	855	PASS
275	198	10	60	23.3	2941	PASS
365	198	1	100	2.0	253	PASS
441	442	0.01	24	16.1	1360	PASS
442	198	50	100	67.0	8440	PASS
443	442	15	24	20.0	1691	PASS