
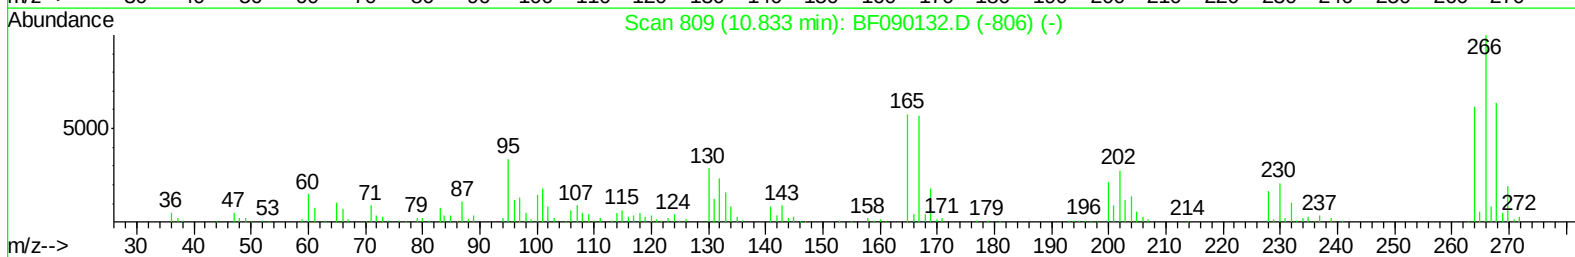
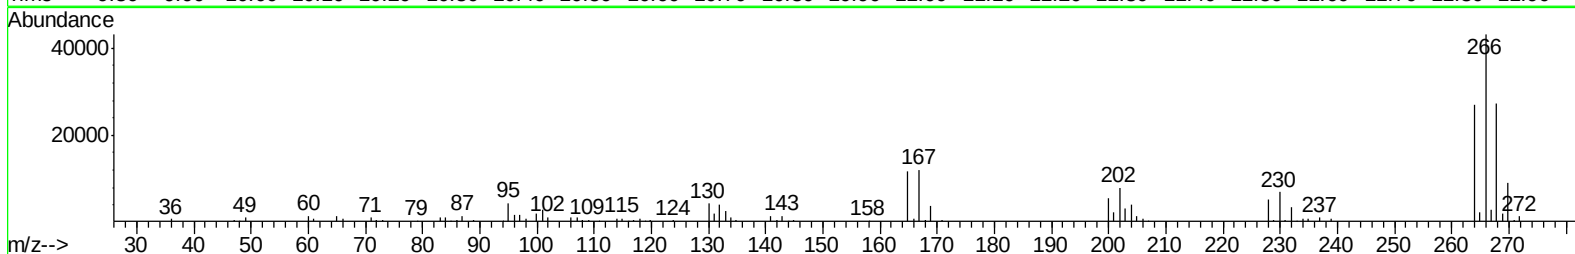


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092116\
Data File : BF090153.D
Acq On : 21 Sep 2016 10:43
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 08:41:03 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 17:58:29 2016
Response via : Initial Calibration

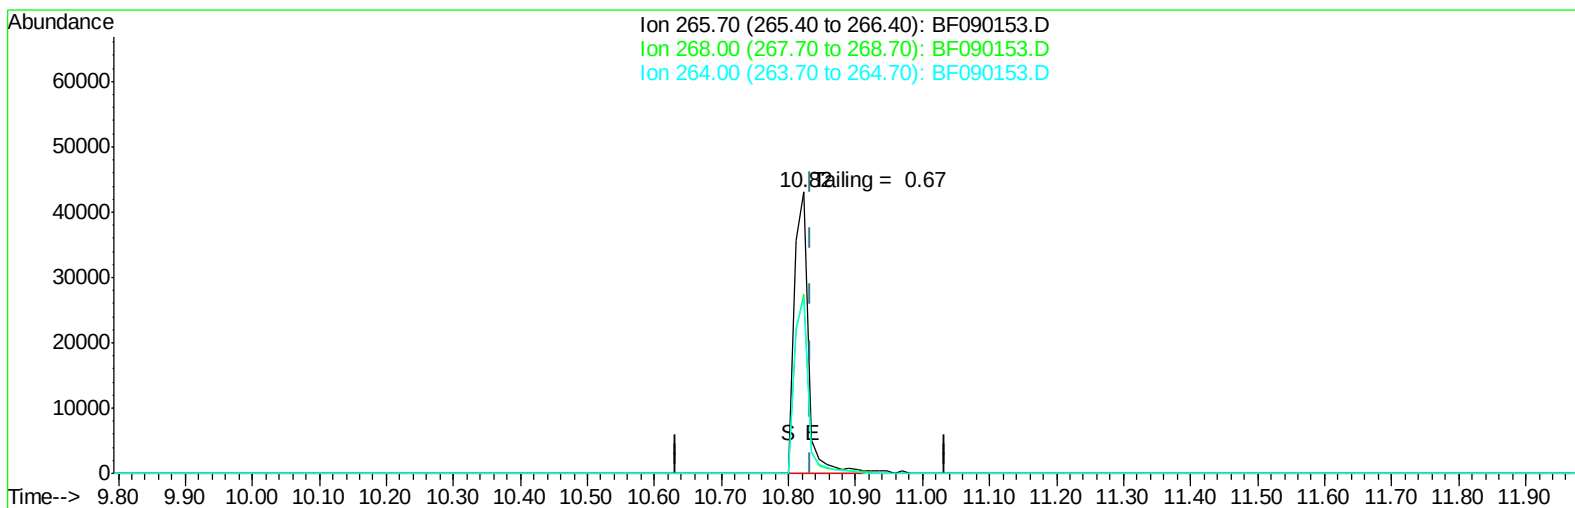

TIC: BF090153.D

(69) Pentachlorophenol (C)




10.822min (-0.011) 0.00ng

response 63124

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	63.44
264.00	62.90	62.33
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092116\
Data File : BF090153.D
Acq On : 21 Sep 2016 10:43
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 08:41:03 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 17:58:29 2016
Response via : Initial Calibration

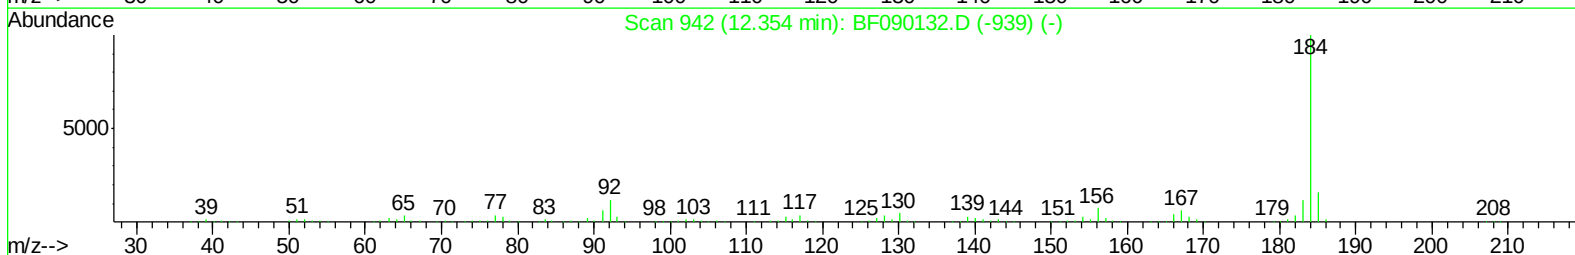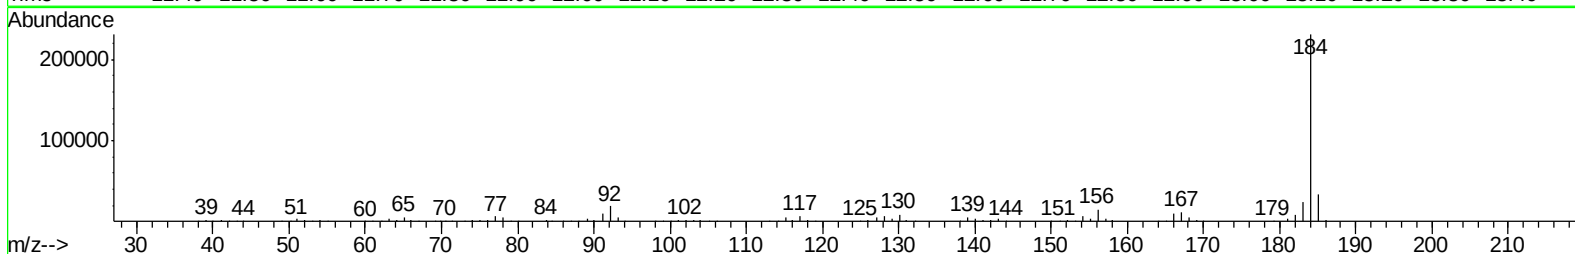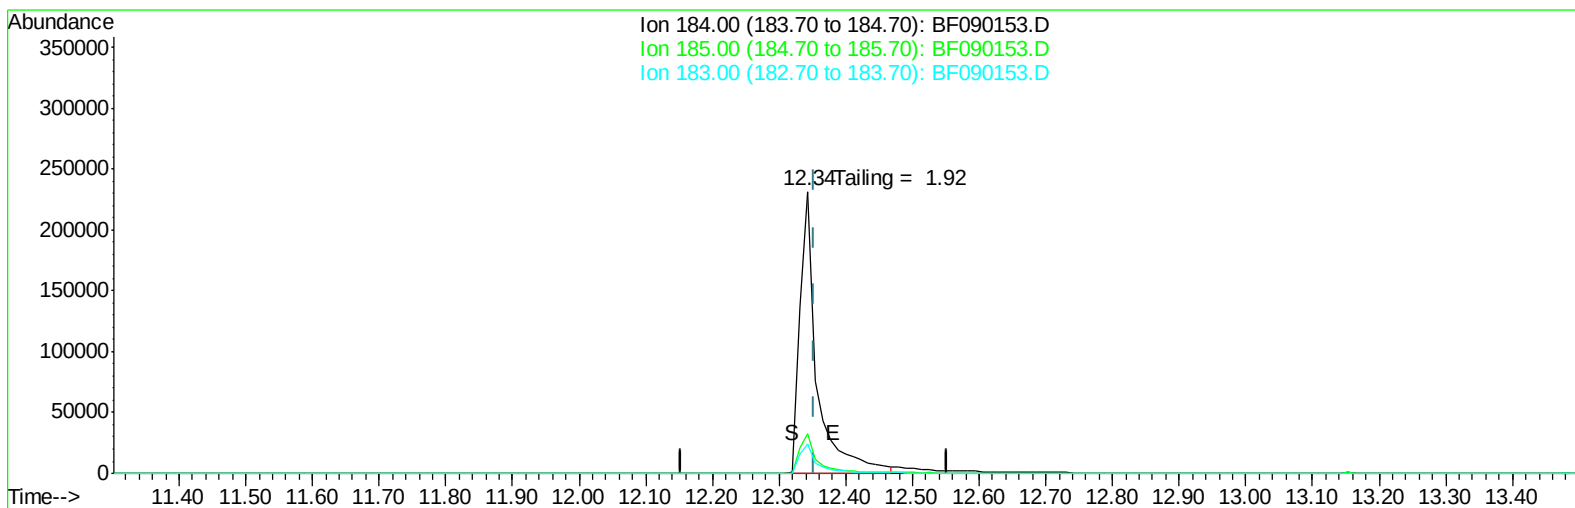

TIC: BF090153.D

(76) Benzidine

12.342min (-0.011) 0.00ng

response 422227

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	14.26
183.00	11.50	10.65
0.00	0.00	0.00