


Data Path : Z:\HPCHEM1\BNA F\DATA\BF092116\
 Data File : BF090153.D
 Acq On : 21 Sep 2016 10:43
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 20 17:58:29 2016

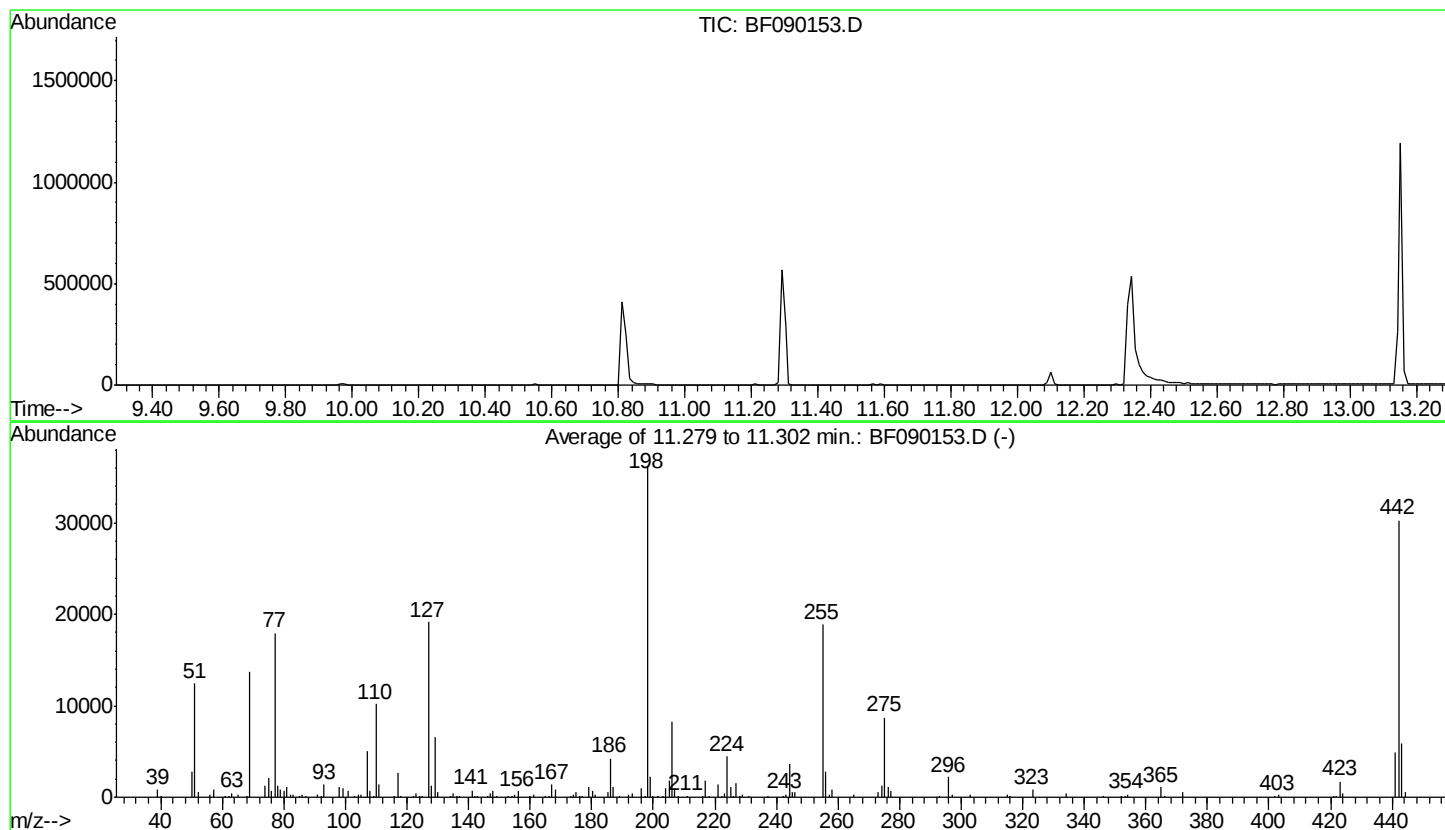

AutoFind: Scans 848, 849, 850; Background Corrected with Scan 845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	12442	PASS
68	69	0.00	2	1.2	160	PASS
69	198	0.00	100	37.9	13742	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.9	19169	PASS
197	198	0.00	2	0.4	141	PASS
198	198	100	100	100.0	36257	PASS
199	198	5	9	6.2	2248	PASS
275	198	10	60	24.0	8696	PASS
365	198	1	100	2.9	1061	PASS
441	442	0.01	24	16.0	4862	PASS
442	198	50	100	83.6	30304	PASS
443	442	15	24	19.3	5857	PASS