


Data Path : Z:\HPCHEM1\BNA F\DATA\BF092116\
 Data File : BF090165.D
 Acq On : 21 Sep 2016 17:24
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 20 17:58:29 2016

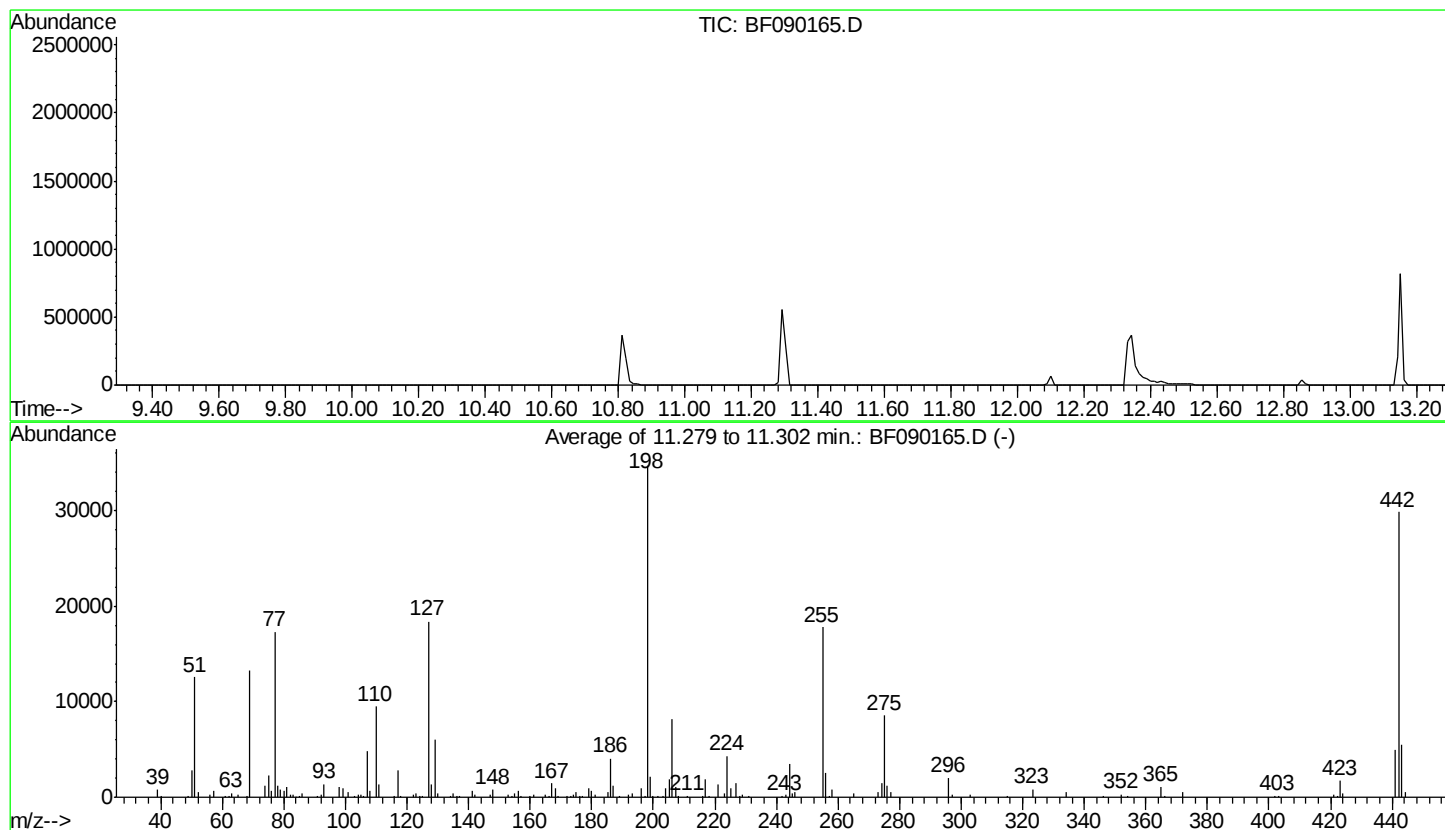

AutoFind: Scans 848, 849, 850; Background Corrected with Scan 845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	12594	PASS
68	69	0.00	2	1.4	185	PASS
69	198	0.00	100	38.1	13242	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.1	18424	PASS
197	198	0.00	2	0.3	110	PASS
198	198	100	100	100.0	34715	PASS
199	198	5	9	6.3	2182	PASS
275	198	10	60	24.6	8542	PASS
365	198	1	100	3.2	1123	PASS
441	442	0.01	24	16.5	4931	PASS
442	198	50	100	86.0	29840	PASS
443	442	15	24	18.6	5542	PASS