
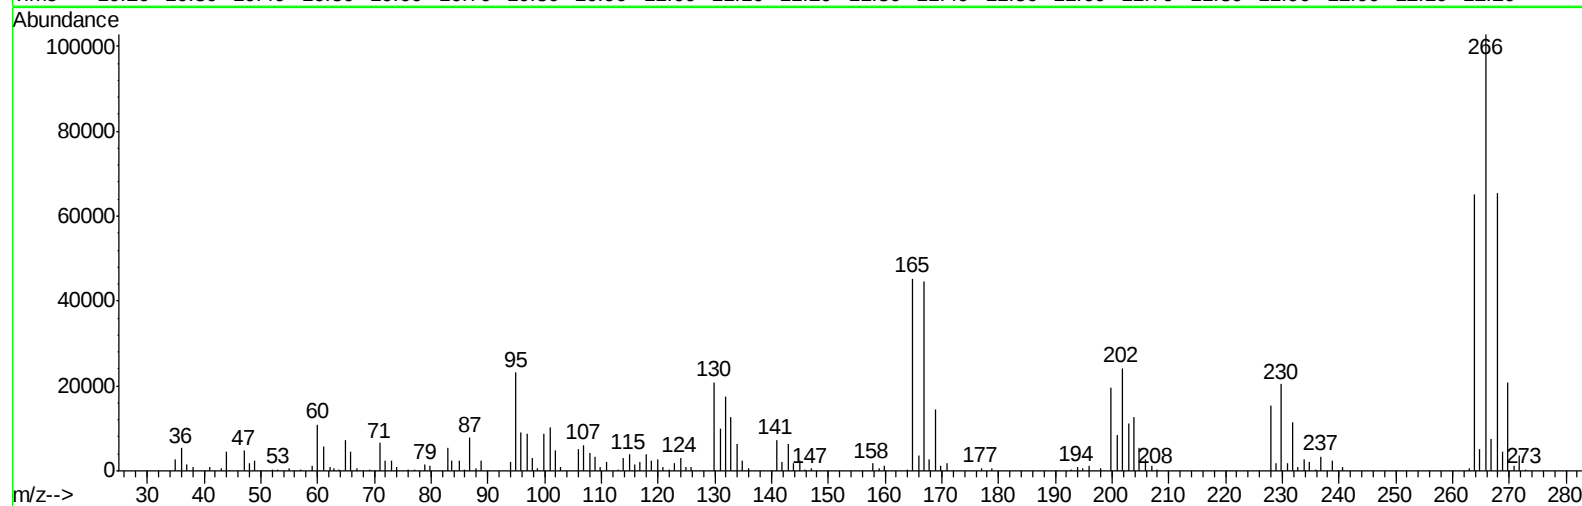


Data Path : Z:\HPCHEM1\BNA F\Data\BF092117\
Data File : BF098675.D
Acq On : 22 Sep 2017 1:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 07:39:57 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 05:59:56 2017
Response via : Initial Calibration

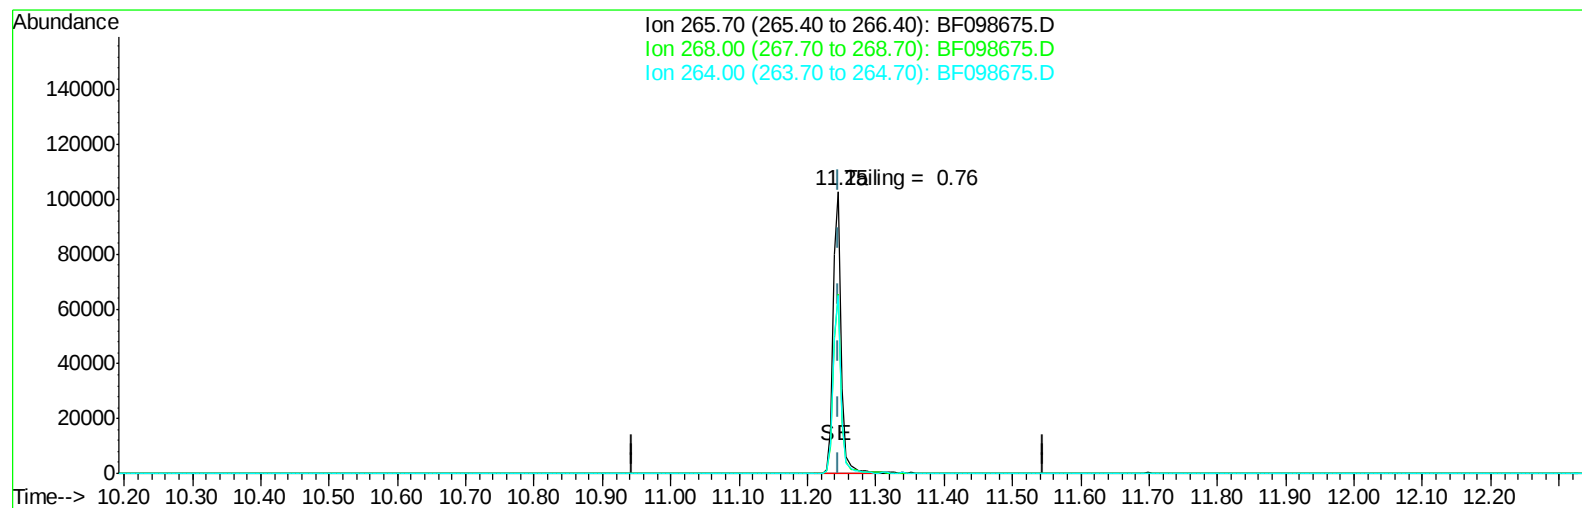

TIC: BF098675.D

(69) Pentachlorophenol (C)



11.245min (+0.000) 31226.72ng

response 87481

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.56
264.00	61.90	63.32
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF092117\
Data File : BF098675.D
Acq On : 22 Sep 2017 1:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 07:39:57 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 05:59:56 2017
Response via : Initial Calibration

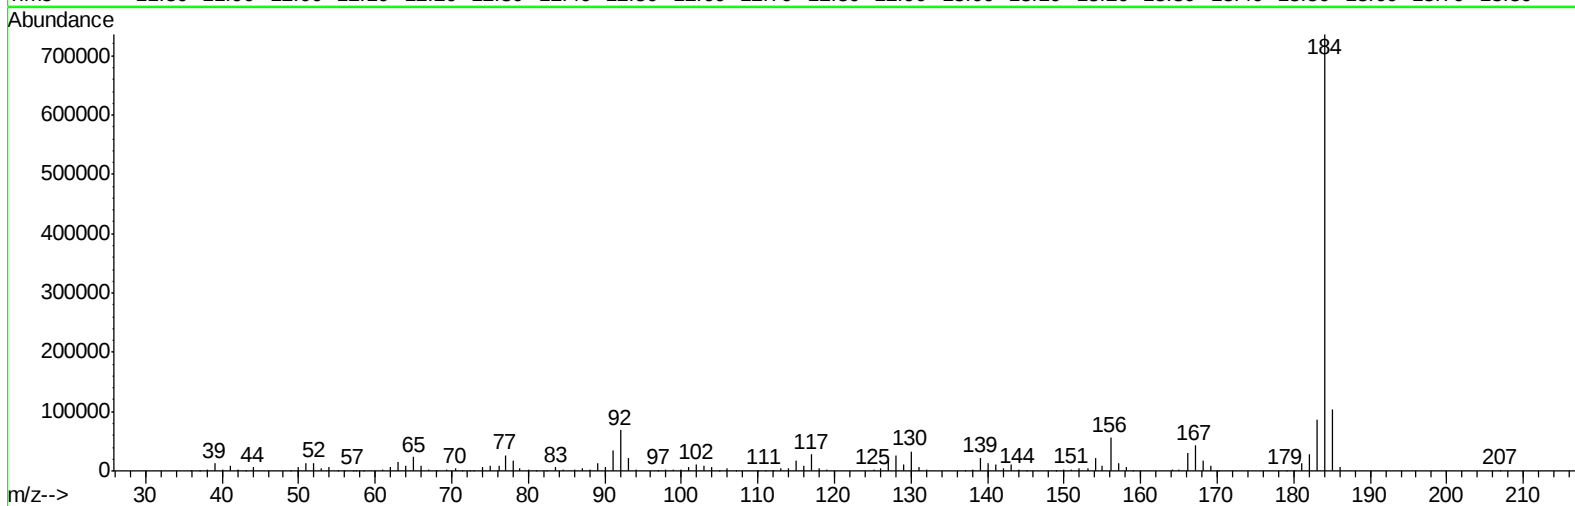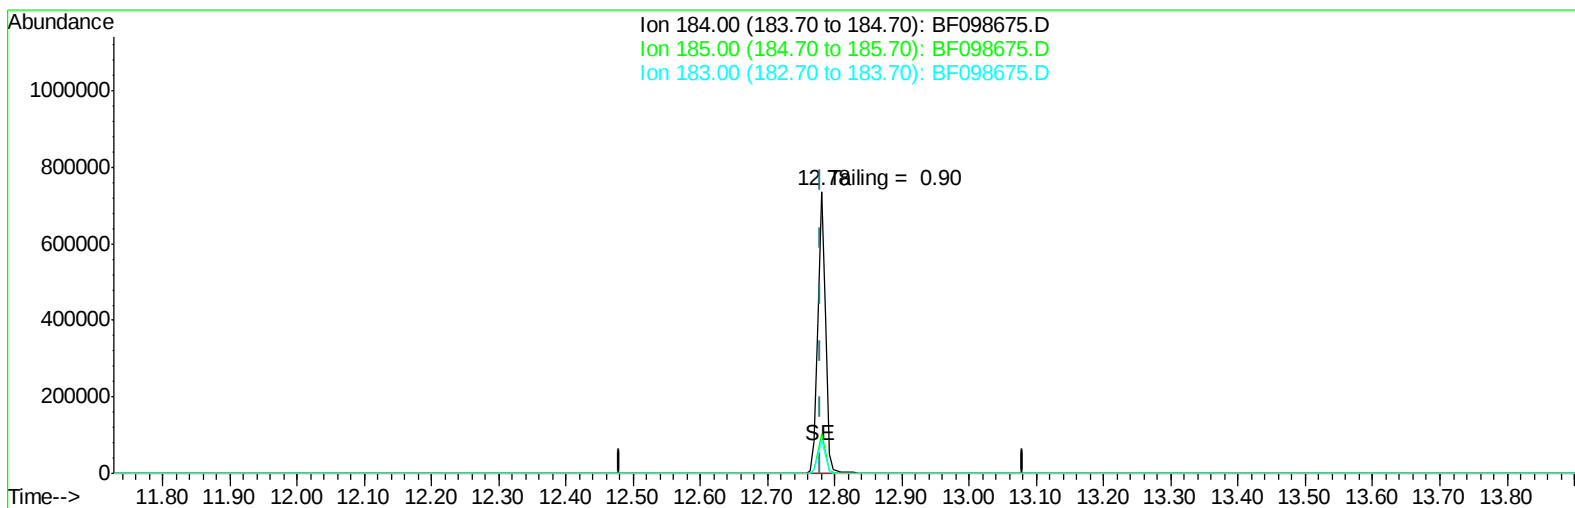

TIC: BF098675.D

(76) Benzidine

12.780min (+0.000) 0.00ng

response 607698

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.15
183.00	11.60	11.88
0.00	0.00	0.00