


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092117\
 Data File : BF098675.D
 Acq On : 22 Sep 2017 1:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 22 10:38:37 2017

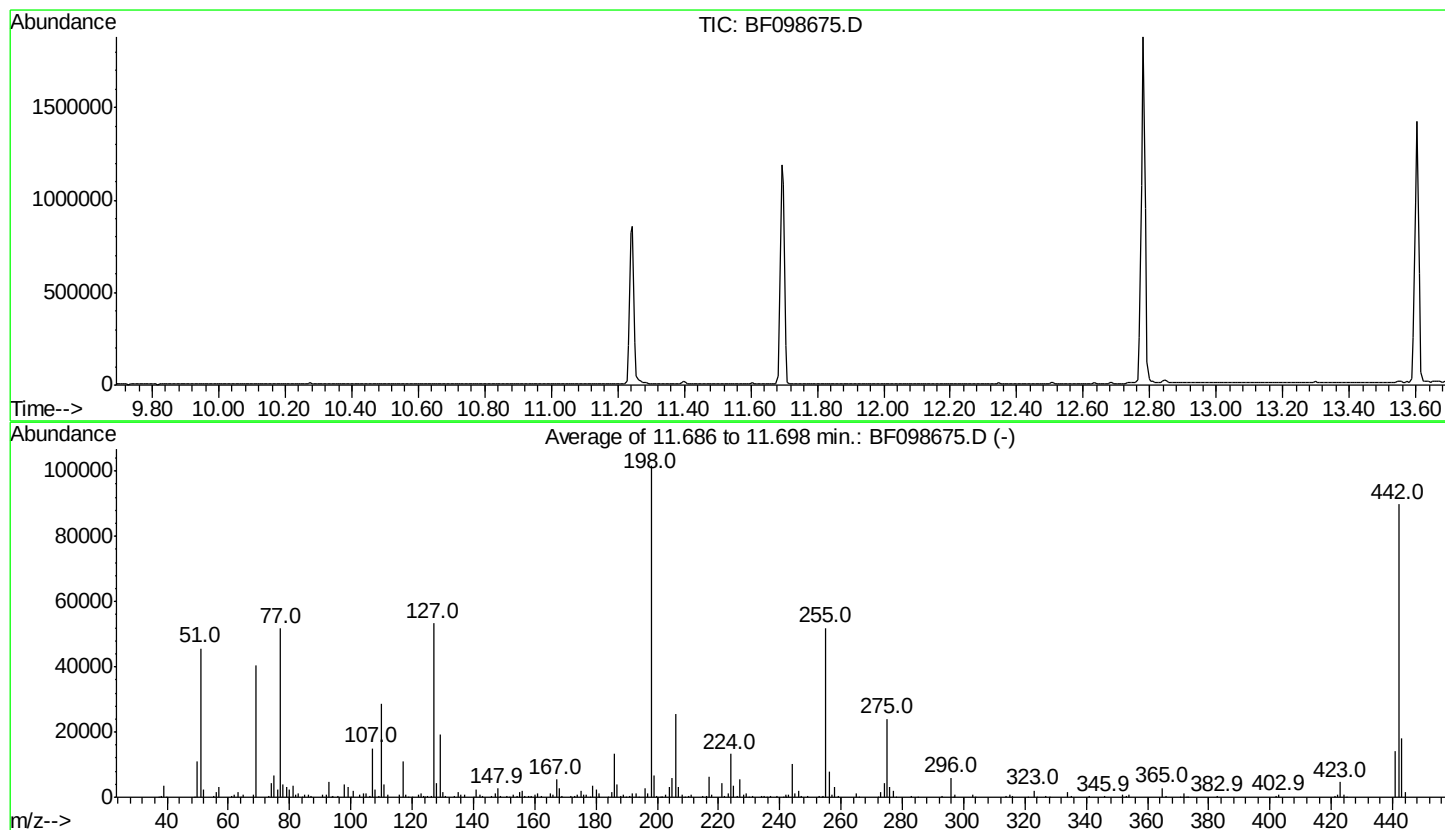

AutoFind: Scans 1632, 1633, 1634; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	45565	PASS
68	69	0.00	2	2.0	814	PASS
69	198	0.00	100	39.8	40472	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.5	53357	PASS
197	198	0.00	2	1.1	1074	PASS
198	198	100	100	100.0	101696	PASS
199	198	5	9	6.6	6748	PASS
275	198	10	60	23.6	23968	PASS
365	198	1	100	2.8	2832	PASS
441	442	0.01	24	15.7	14128	PASS
442	198	50	100	88.3	89752	PASS
443	442	15	24	20.0	17958	PASS