

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092120\
 Data File : BF121623.D
 Acq On : 21 Sep 2020 13:10
 Operator : JU/CG
 Sample : PB131730BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB131730BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.069	503	507	517	rVB	67027	100625	1.50%	0.261%
2	5.451	567	572	575	rBV	4493403	4651225	69.18%	12.084%
3	6.457	737	743	746	rBV	4045880	4770452	70.95%	12.394%
4	6.816	800	804	807	rBV	1305623	1043123	15.51%	2.710%
5	7.381	894	900	903	rBV	2830452	3437223	51.12%	8.930%
6	8.098	1017	1022	1026	rBV	1364195	1376296	20.47%	3.576%
7	9.181	1199	1206	1209	rBV	4894895	5902013	87.78%	15.333%
8	9.857	1315	1321	1325	rBV	1542677	1604370	23.86%	4.168%
9	10.651	1449	1456	1460	rBV	3331908	3887376	57.82%	10.099%
10	11.345	1568	1574	1578	rBV	1642802	1668977	24.82%	4.336%
11	12.945	1838	1846	1849	rBV	6163874	6723401	100.00%	17.467%
12	13.992	2019	2024	2034	rVB	1841946	1691227	25.15%	4.394%
13	15.457	2266	2273	2277	rBV	1249793	1634860	24.32%	4.247%


Sum of corrected areas: 38491168

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092120\
Data File : BF121623.D
Acq On : 21 Sep 2020 13:10
Operator : JU/CG
Sample : PB131730BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131730BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

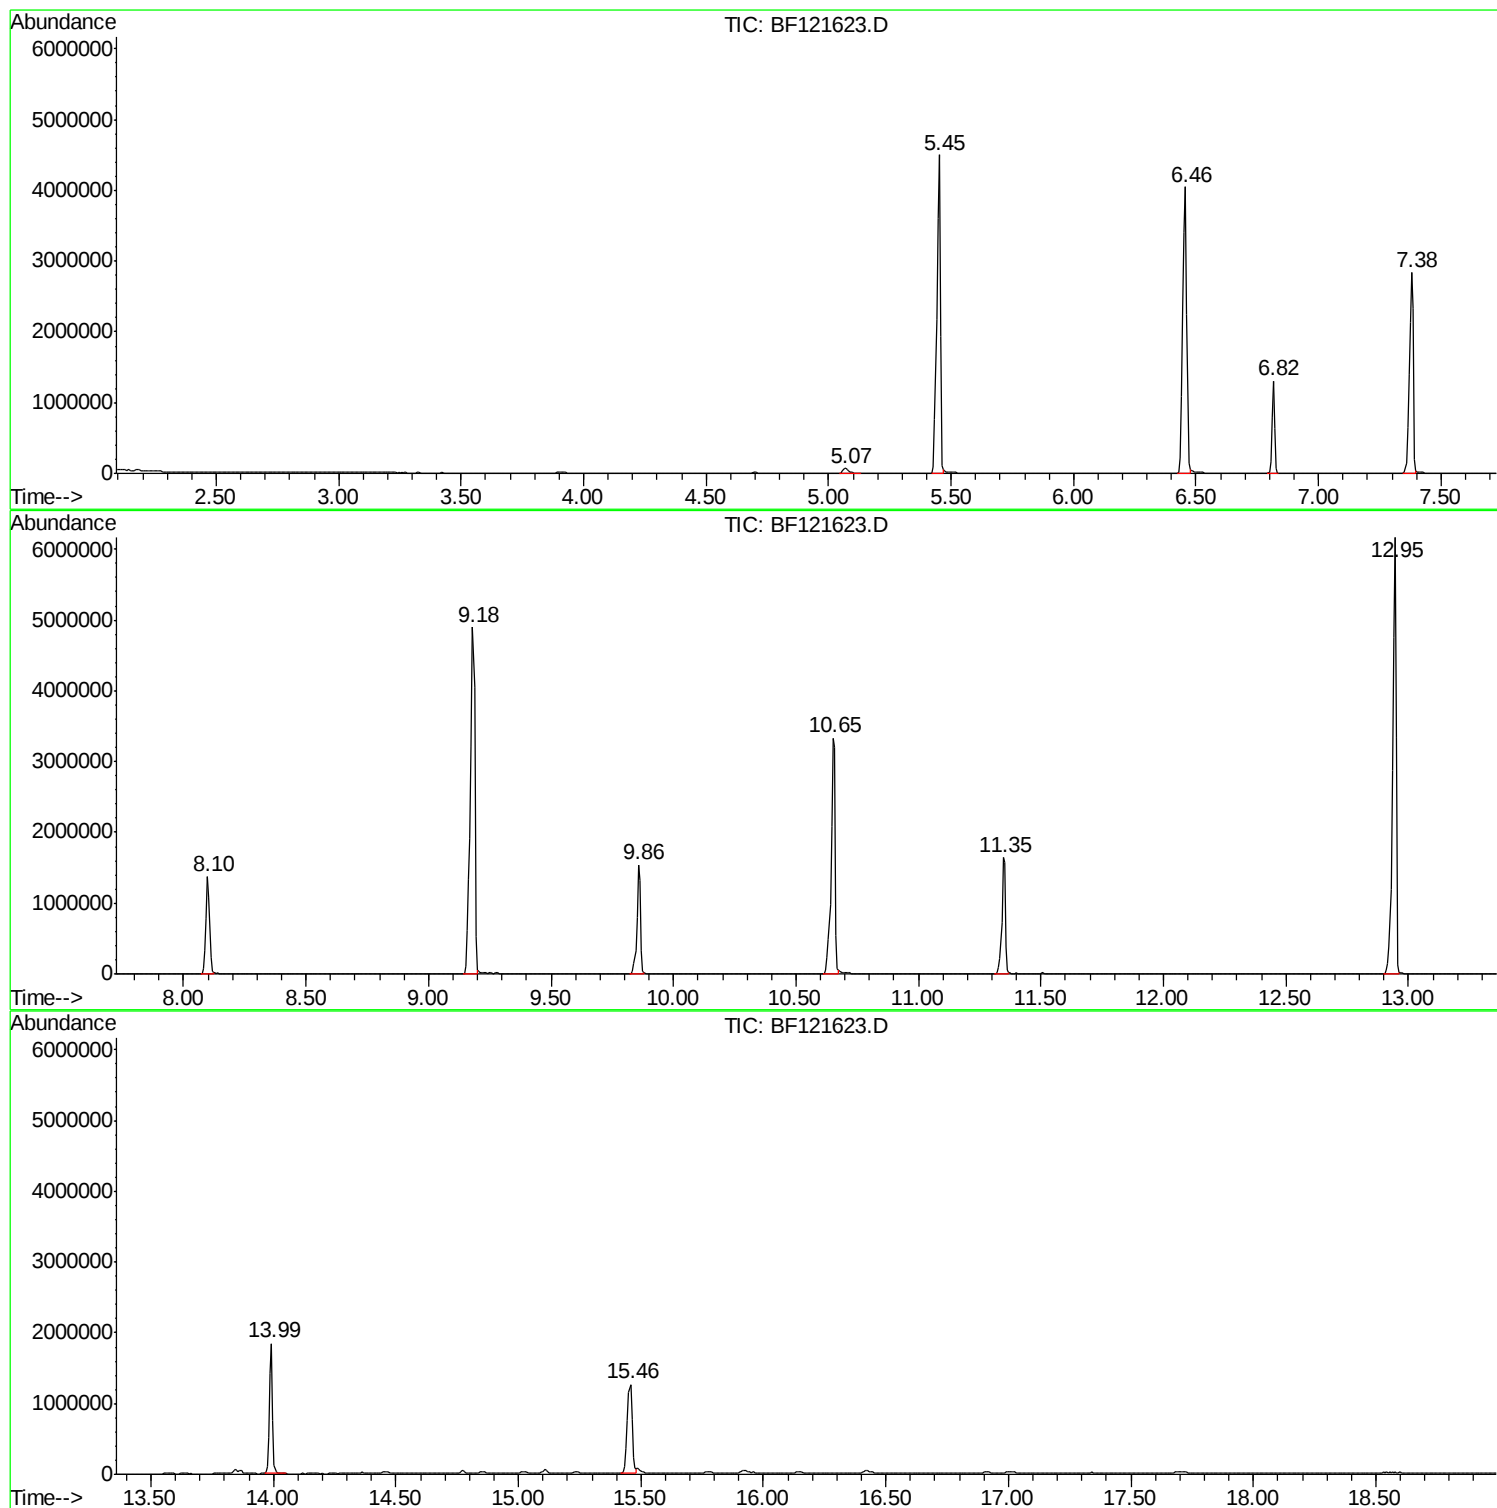

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092120\
Data File : BF121623.D
Acq On : 21 Sep 2020 13:10
Operator : JU/CG
Sample : PB131730BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131730BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092120\
Data File : BF121623.D
Acq On : 21 Sep 2020 13:10
Operator : JU/CG
Sample : PB131730BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131730BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc