


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092120\
 Data File : BF121621.D
 Acq On : 21 Sep 2020 11:56
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 21 14:19:01 2020

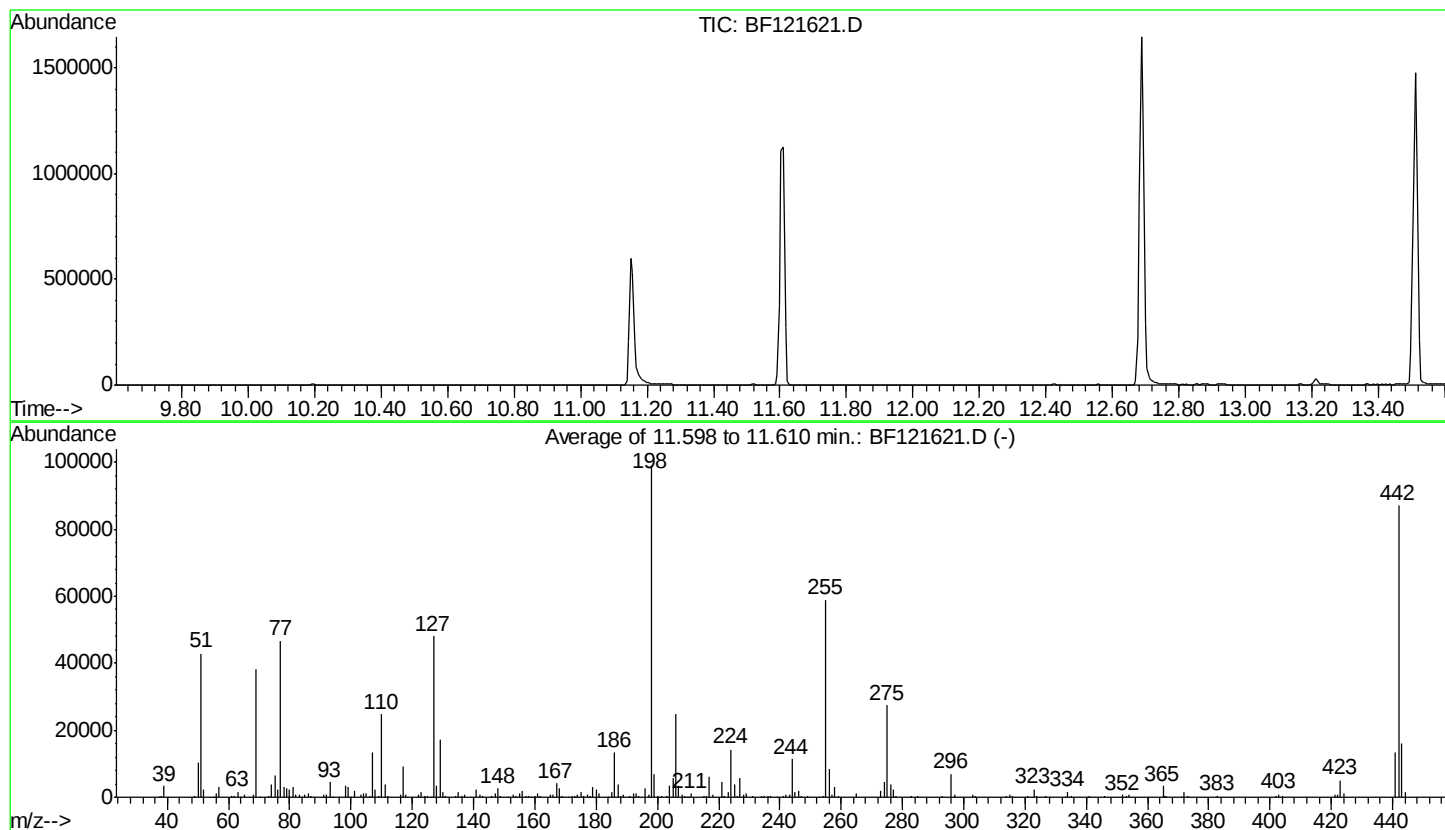

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	42936	PASS
68	69	0.00	2	1.9	747	PASS
69	198	0.00	100	38.8	38384	PASS
70	69	0.00	2	0.3	115	PASS
127	198	10	80	48.6	48064	PASS
197	198	0.00	2	0.8	824	PASS
198	198	100	100	100.0	98994	PASS
199	198	5	9	6.9	6866	PASS
275	198	10	60	27.7	27407	PASS
365	198	1	100	3.4	3386	PASS
441	198	0.01	100	13.7	13555	PASS
442	198	50	100	87.9	87010	PASS
443	442	15	24	18.3	15941	PASS