
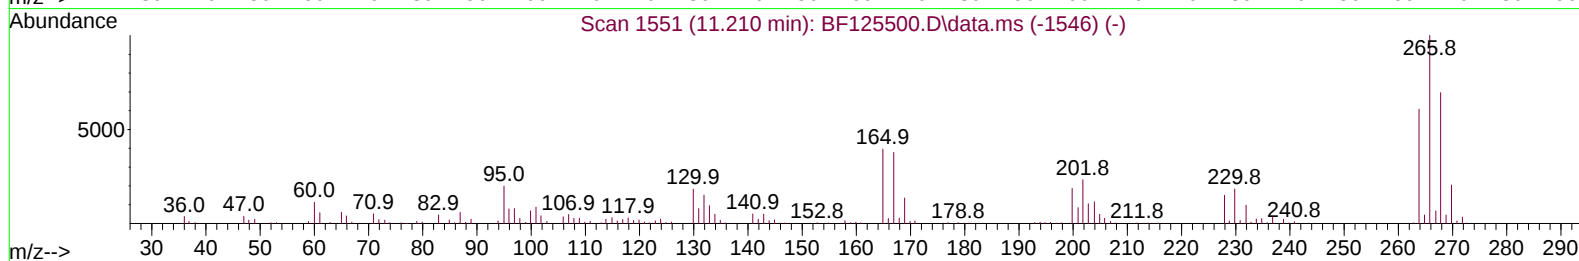
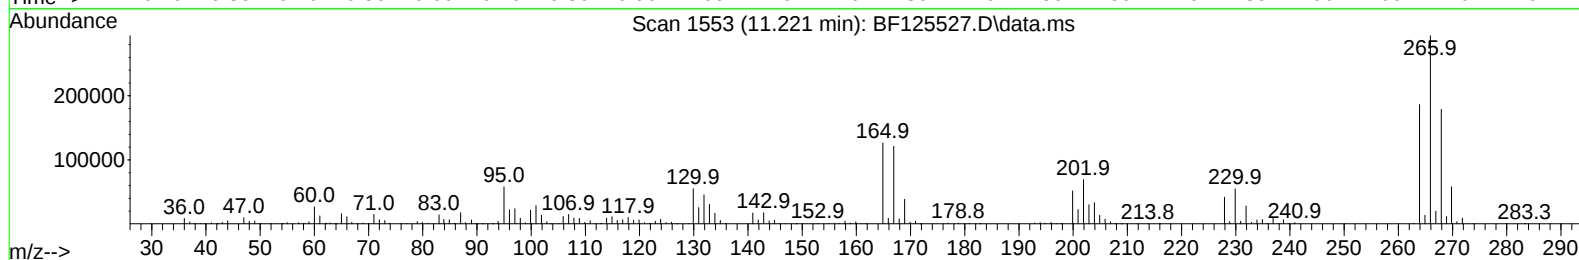


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092121\
Data File : BF125527.D
Acq On : 21 Sep 2021 9:42
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 12:49:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 12:45:25 2021
Response via : Initial Calibration

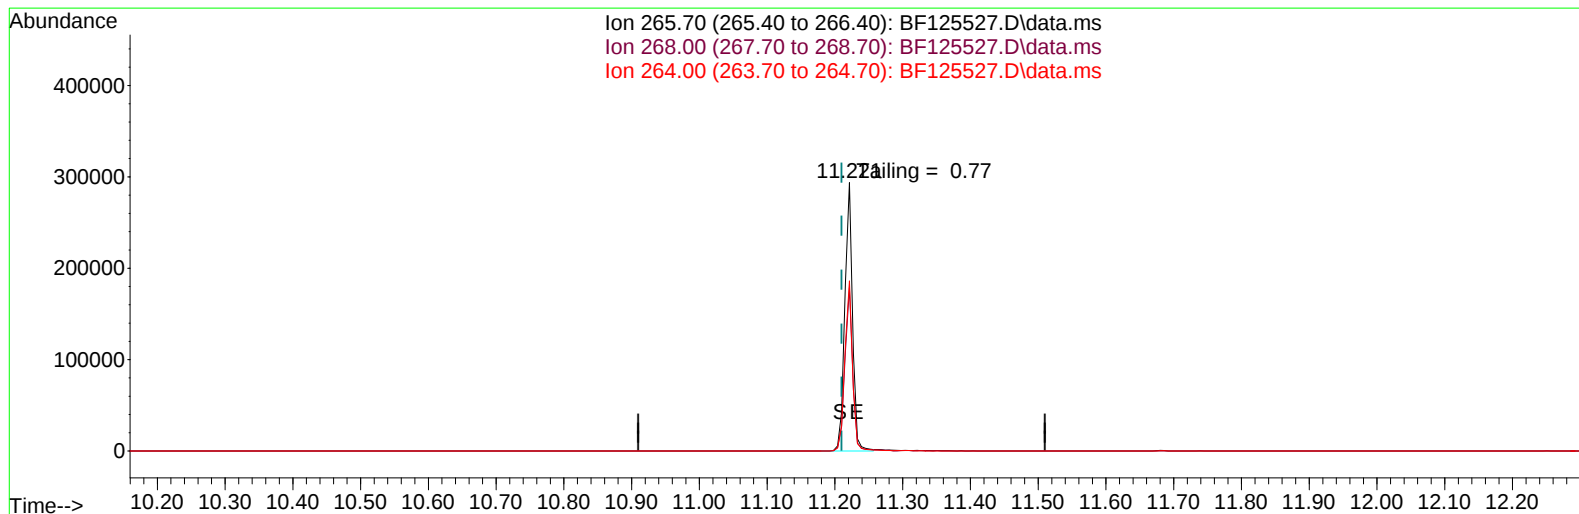

TIC: BF125527.D\data.ms

(70) Pentachlorophenol (C)




11.221min (+ 0.012) 0.00 ng

response 234892

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	60.88
264.00	69.90	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092121\
 Data File : BF125527.D
 Acq On : 21 Sep 2021 9:42
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 12:49:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 21 12:45:25 2021
 Response via : Initial Calibration

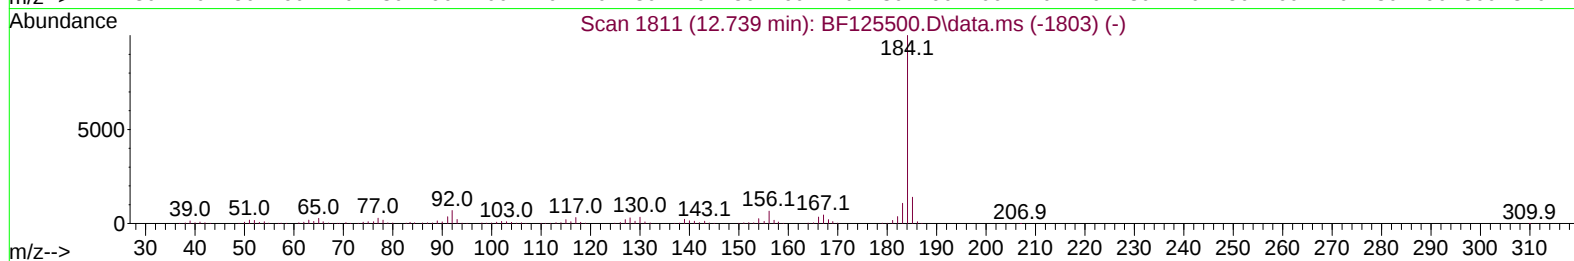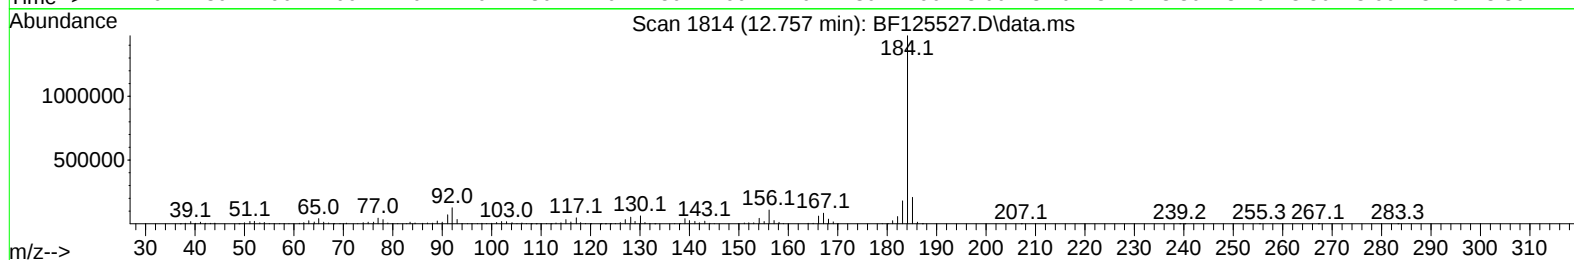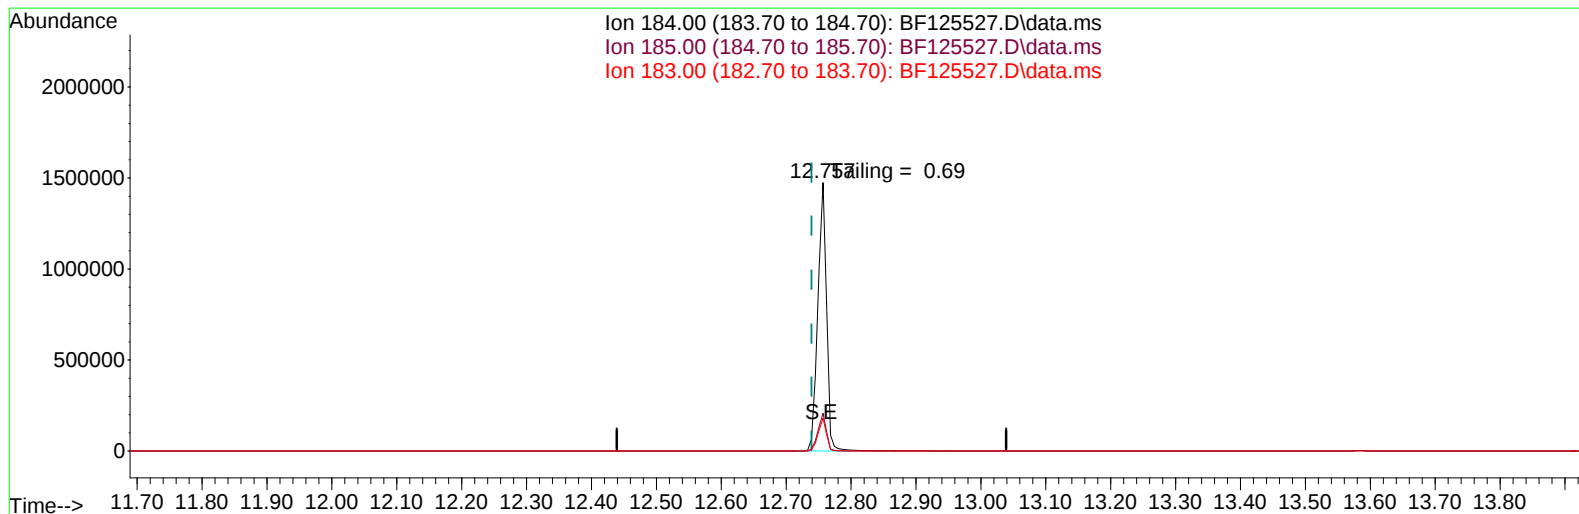

TIC: BF125527.D\data.ms

(77) Benzidine

12.757min (+ 0.018) 202540.19 ng

response 1392459

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.07
183.00	10.10	12.22#
0.00	0.00	0.00