

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092121\
 Data File : BF125543.D
 Acq On : 21 Sep 2021 19:07
 Operator : JU/CG
 Sample : M3835-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SW-CB-02-(0.2)

Quant Time: Sep 22 04:02:26 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 21 19:21:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.892	152	210396	20.000	ng	0.00
21) Naphthalene-d8	8.175	136	875289	20.000	ng	# 0.00
39) Acenaphthene-d10	9.933	164	473515	20.000	ng	0.00
64) Phenanthrene-d10	11.416	188	815140	20.000	ng	# 0.00
76) Chrysene-d12	14.051	240	473292	20.000	ng	-0.01
86) Perylene-d12	15.533	264	399981	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.510	112	801429	60.236	ng	0.00
7) Phenol-d6	6.504	99	598171	34.870	ng	-0.02
23) Nitrobenzene-d5	7.457	82	1256014	91.525	ng	0.00
42) 2,4,6-Tribromophenol	10.721	330	594257	128.130	ng	0.00
45) 2-Fluorobiphenyl	9.257	172	2397324	92.676	ng	0.00
79) Terphenyl-d14	13.010	244	2421026	82.603	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092121\
Data File : BF125543.D
Acq On : 21 Sep 2021 19:07
Operator : JU/CG
Sample : M3835-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-CB-02-(0.2)

Quant Time: Sep 22 04:02:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 19:21:36 2021
Response via : Initial Calibration




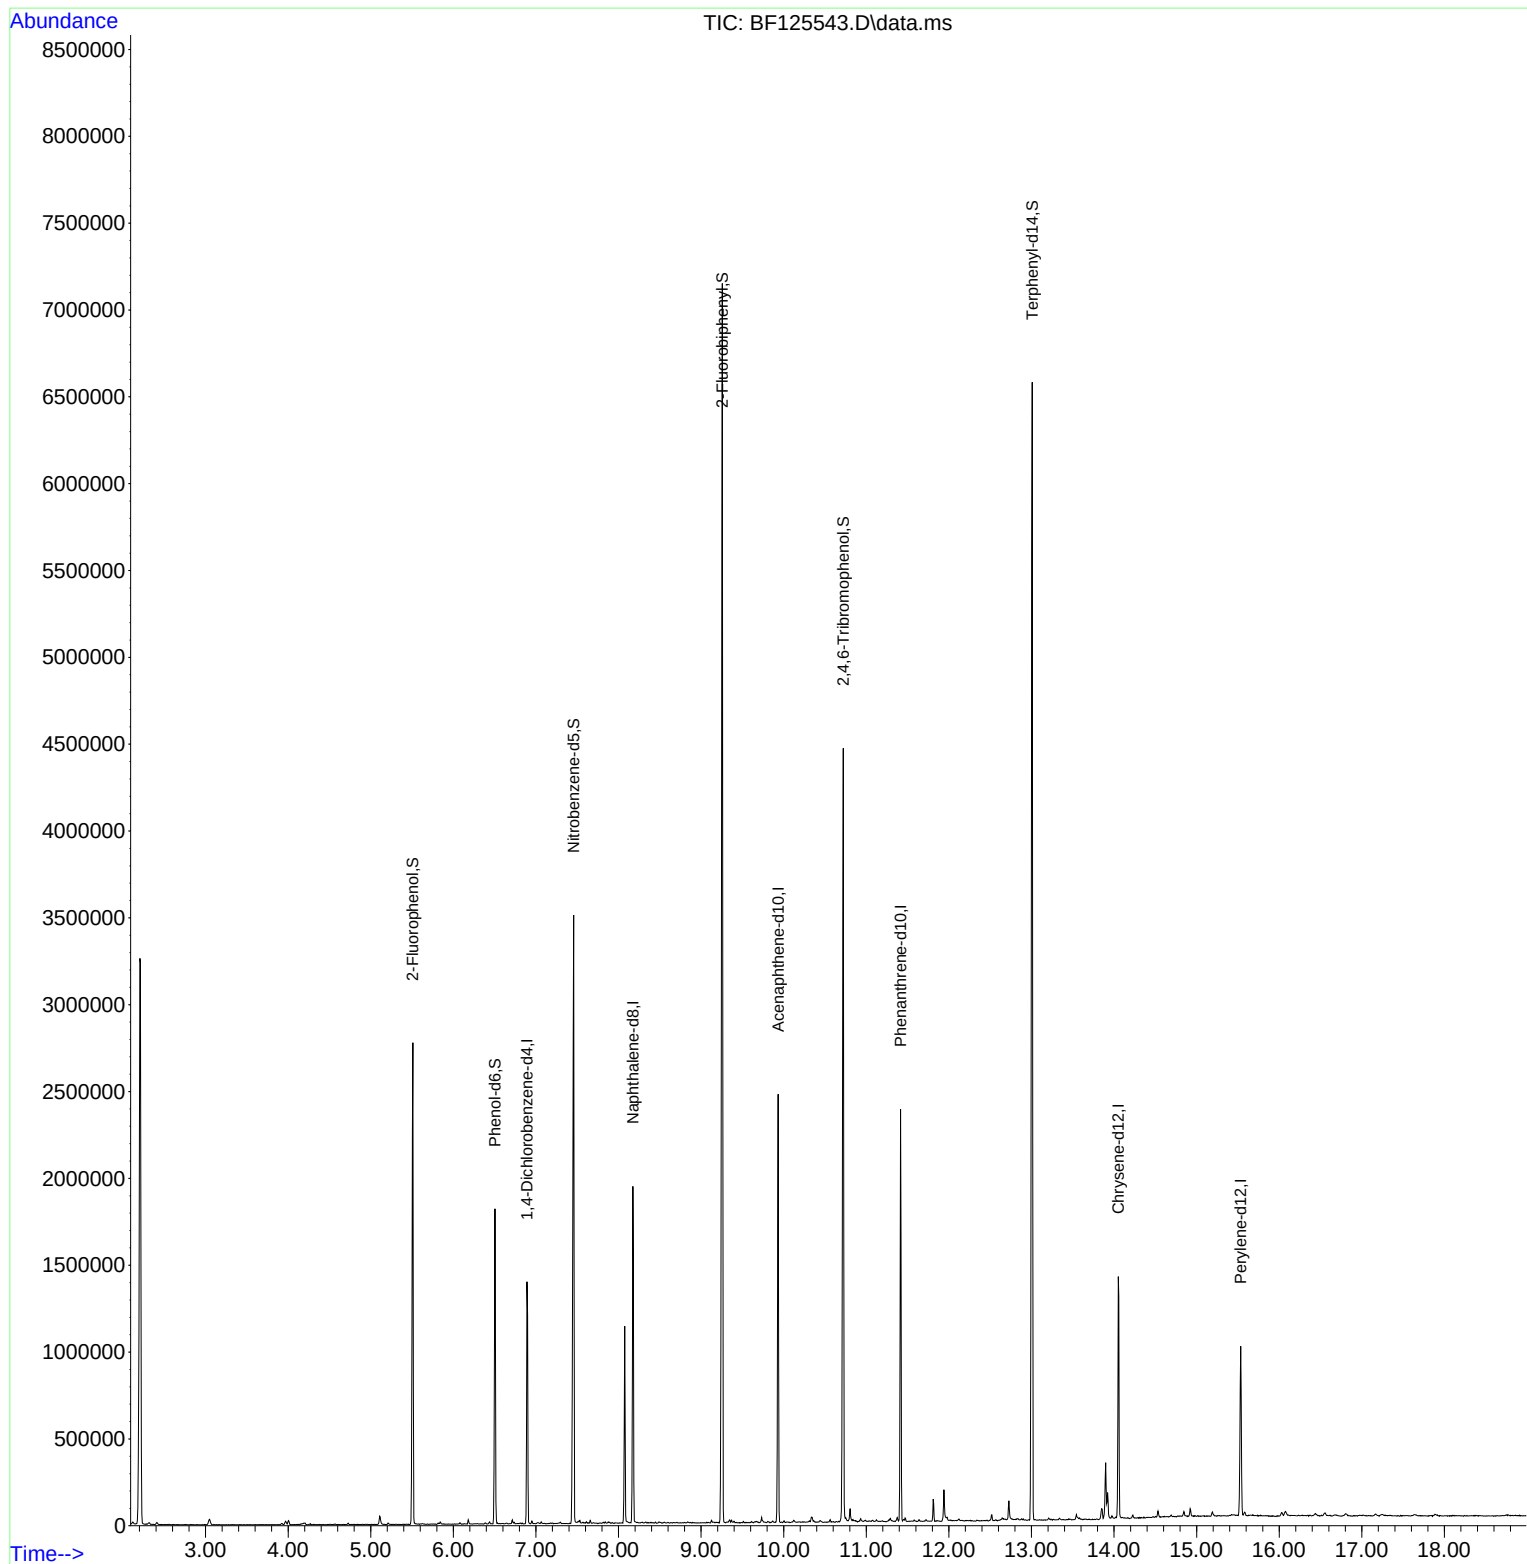


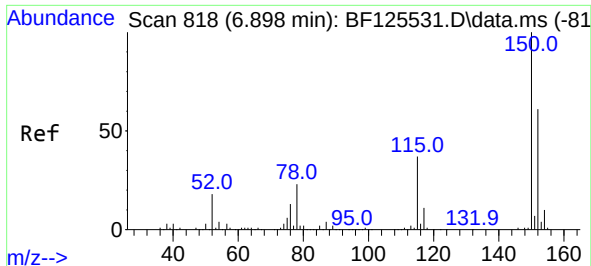

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.892 min Scan# 817
Delta R.T. -0.006 min
Lab File: BF125543.D
Acq: 21 Sep 2021 19:07




Instrument :
BNA_F
ClientSampleId :
SW-CB-02-(0.2)


Tgt Ion:152 Resp: 210396
Ion Ratio Lower Upper
152 100
150 162.3 117.6 176.4
115 61.3 47.1 70.7

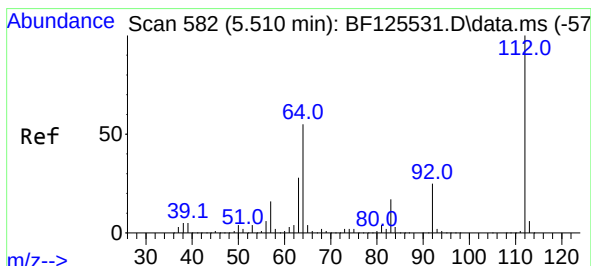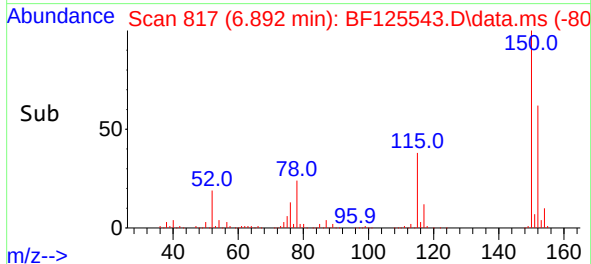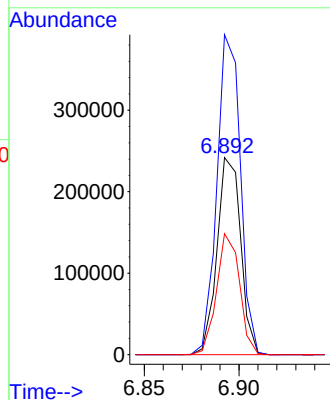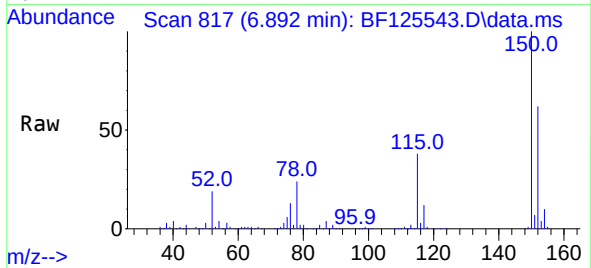

#5
2-Fluorophenol
Concen: 60.236 ng
RT: 5.510 min Scan# 582
Delta R.T. 0.000 min
Lab File: BF125543.D
Acq: 21 Sep 2021 19:07

Tgt Ion:112 Resp: 801429
Ion Ratio Lower Upper
112 100
64 52.9 44.2 66.2
63 26.3 26.2 39.2


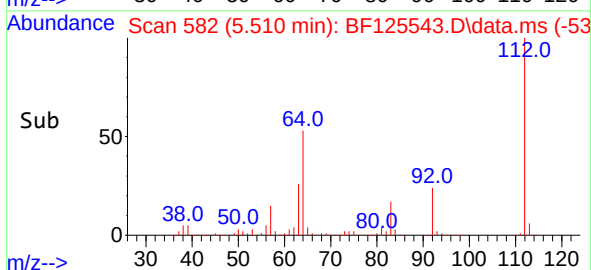
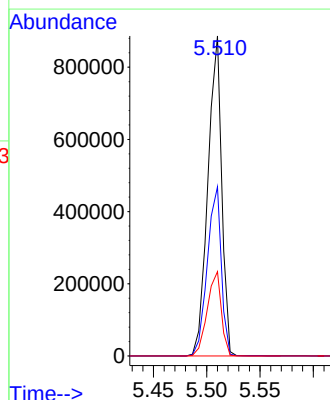
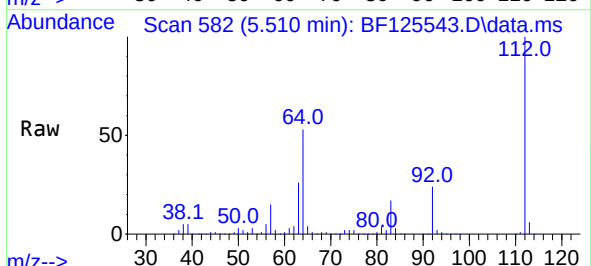


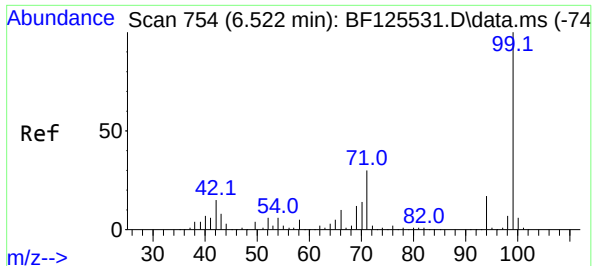

#7
Phenol-d6
Concen: 34.870 ng
RT: 6.504 min Scan# 751
Delta R.T. -0.018 min
Lab File: BF125543.D
Acq: 21 Sep 2021 19:07




Instrument :
BNA_F
ClientSampleId :
SW-CB-02-(0.2)


Tgt Ion: 99 Resp: 598171
Ion Ratio Lower Upper
99 100
42 15.7 23.5 35.3#
71 29.4 25.6 38.4

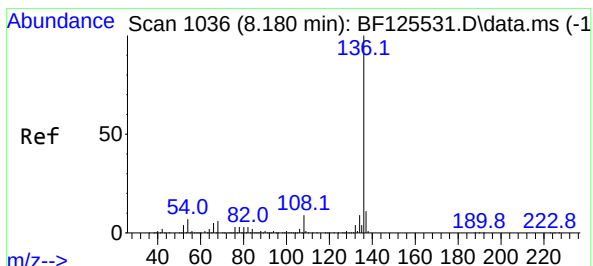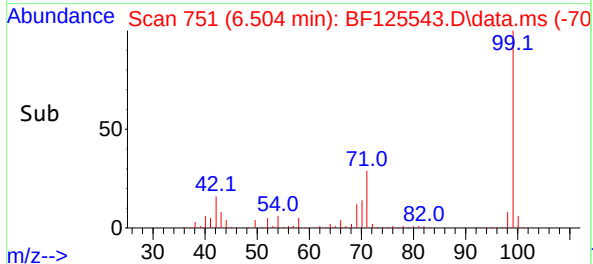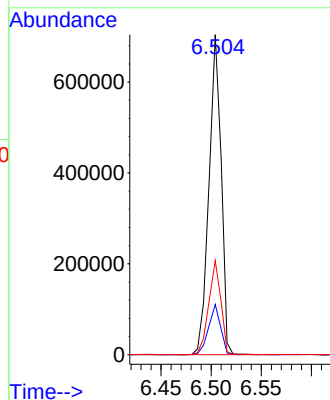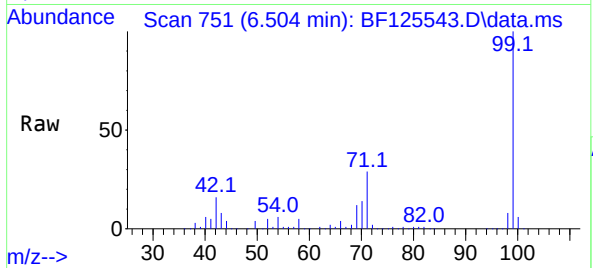

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.175 min Scan# 1035
Delta R.T. -0.006 min
Lab File: BF125543.D
Acq: 21 Sep 2021 19:07

Tgt Ion:136 Resp: 875289
Ion Ratio Lower Upper
136 100
137 10.6 9.8 14.6
54 7.0 6.4 9.6
68 5.8 3.3 4.9#


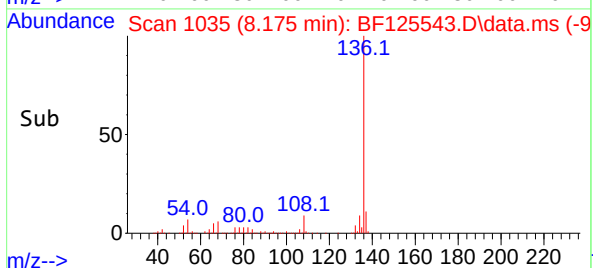
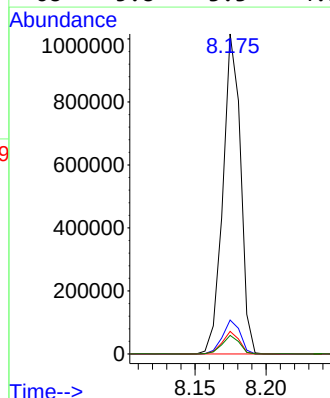
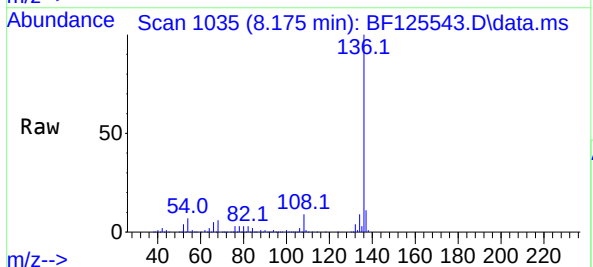


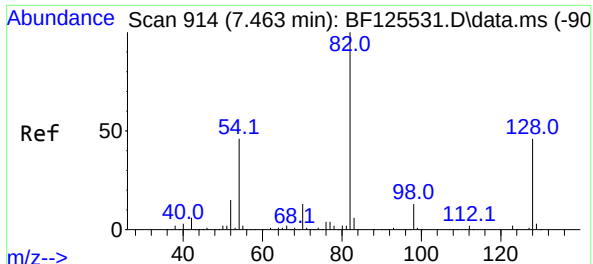

#23
Nitrobenzene-d5
Concen: 91.525 ng
RT: 7.457 min Scan# 913
Delta R.T. -0.006 min
Lab File: BF125543.D
Acq: 21 Sep 2021 19:07




Instrument :
BNA_F
ClientSampleId :
SW-CB-02-(0.2)


Tgt Ion: 82 Resp: 1256014
Ion Ratio Lower Upper
82 100
128 47.3 40.6 60.8
54 46.4 49.6 74.4#

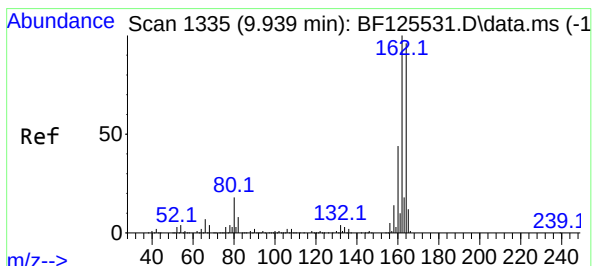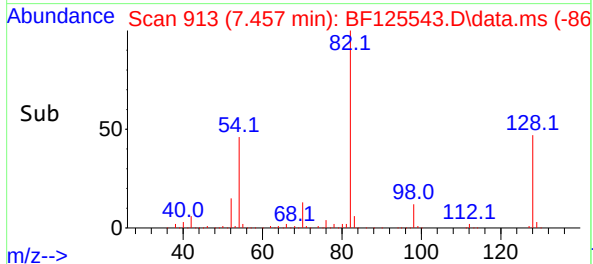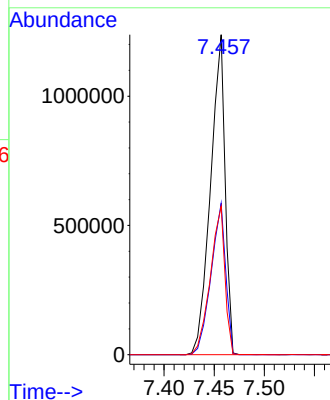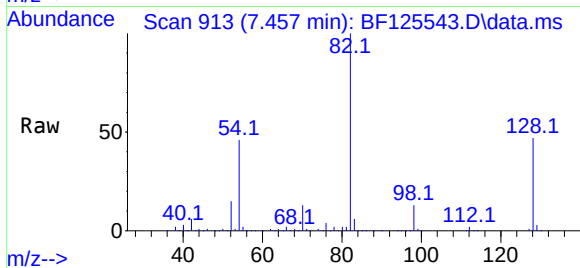

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.933 min Scan# 1334
Delta R.T. -0.006 min
Lab File: BF125543.D
Acq: 21 Sep 2021 19:07

Tgt Ion: 164 Resp: 473515
Ion Ratio Lower Upper
164 100
162 103.7 81.3 121.9
160 45.2 38.0 57.0


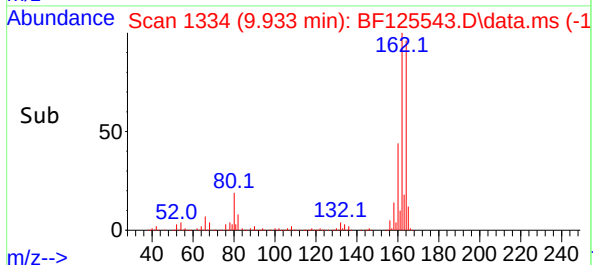
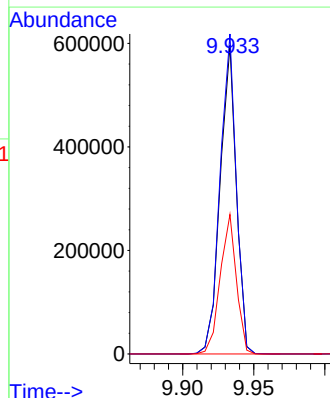
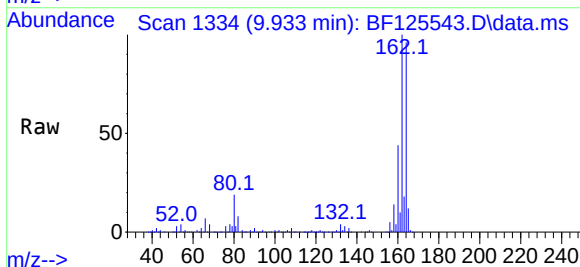


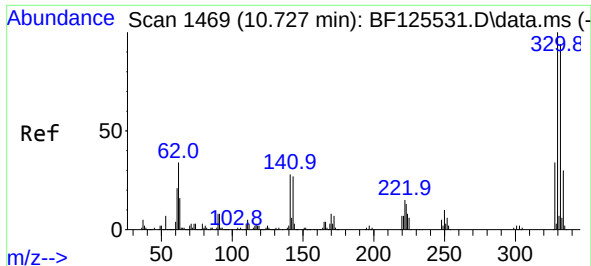

#42
2,4,6-Tribromophenol
Concen: 128.130 ng
RT: 10.721 min Scan# 1468
Delta R.T. -0.006 min
Lab File: BF125543.D
Acq: 21 Sep 2021 19:07




Instrument :
BNA_F
ClientSampleId :
SW-CB-02-(0.2)


Tgt Ion:330 Resp: 594257
Ion Ratio Lower Upper
330 100
332 93.5 76.2 114.4
141 31.8 44.6 66.8#

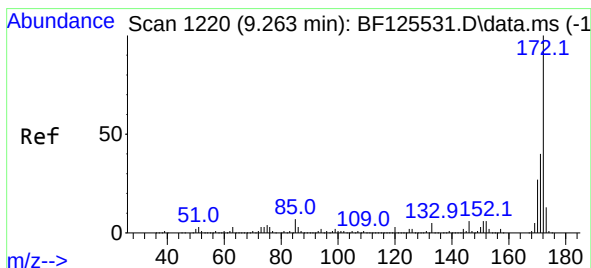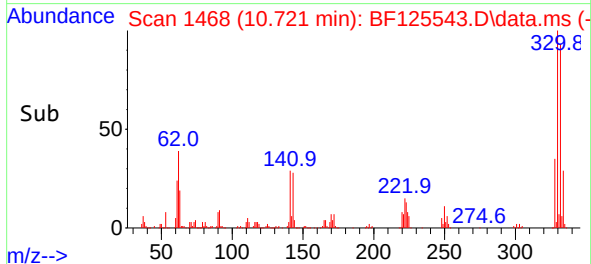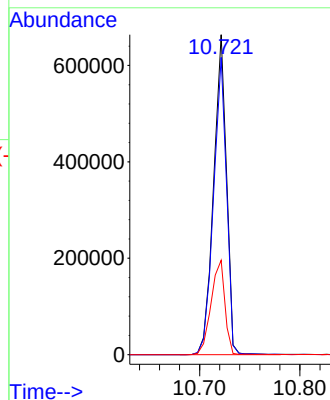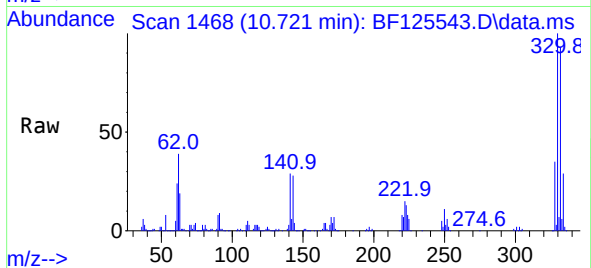

#45
2-Fluorobiphenyl
Concen: 92.676 ng
RT: 9.257 min Scan# 1219
Delta R.T. -0.006 min
Lab File: BF125543.D
Acq: 21 Sep 2021 19:07

Tgt Ion:172 Resp: 2397324
Ion Ratio Lower Upper
172 100
171 40.6 26.5 39.7#
170 27.0 18.8 28.2


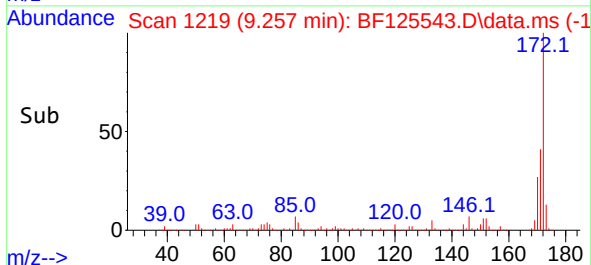
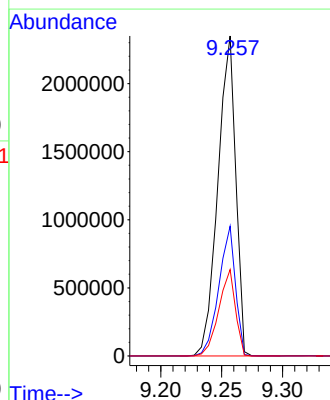
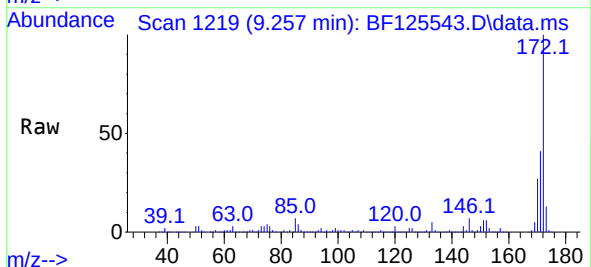


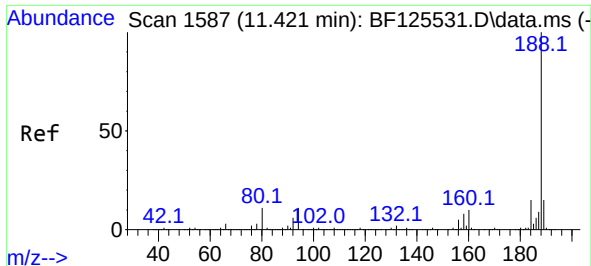

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.416 min Scan# 1586
Delta R.T. -0.006 min
Lab File: BF125543.D
Acq: 21 Sep 2021 19:07




Instrument :
BNA_F
ClientSampleId :
SW-CB-02-(0.2)


Tgt Ion:188 Resp: 815140
Ion Ratio Lower Upper
188 100
94 10.1 6.7 10.1#
80 10.7 7.5 11.3

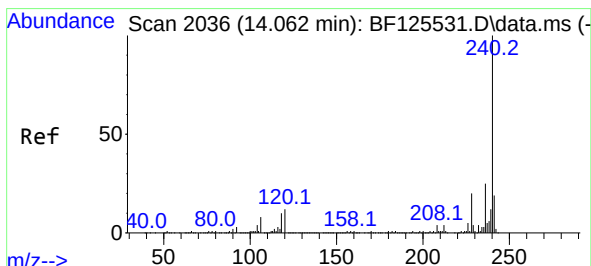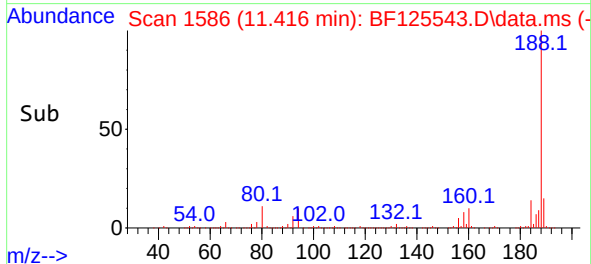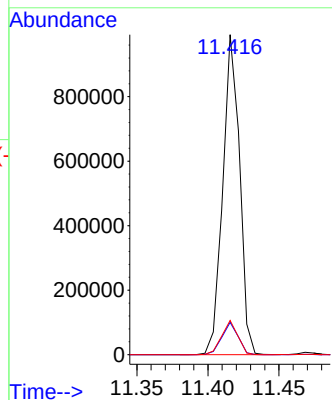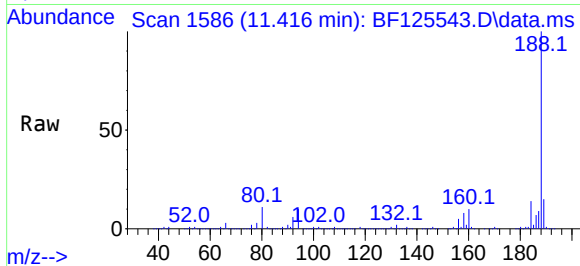

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.051 min Scan# 2034
Delta R.T. -0.012 min
Lab File: BF125543.D
Acq: 21 Sep 2021 19:07

Tgt Ion:240 Resp: 473292
Ion Ratio Lower Upper
240 100
120 13.4 10.8 16.2
236 25.8 21.6 32.4


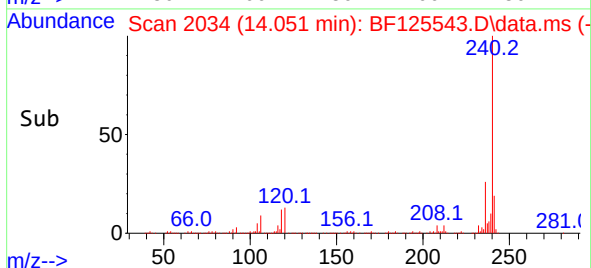
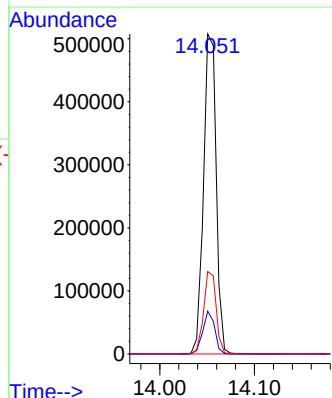
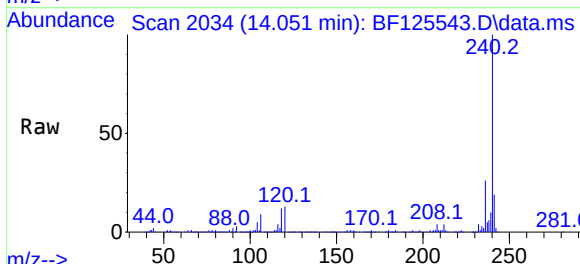


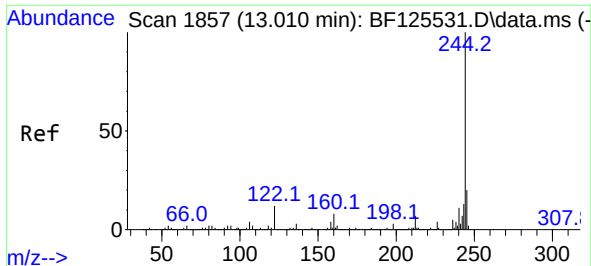

#79
Terphenyl-d14
Concen: 82.603 ng
RT: 13.010 min Scan# 1857
Delta R.T. 0.000 min
Lab File: BF125543.D
Acq: 21 Sep 2021 19:07

Instrument :
BNA_F
ClientSampleId :
SW-CB-02-(0.2)

Tgt Ion:244 Resp: 2421026
Ion Ratio Lower Upper
244 100
212 7.4 5.9 8.9
122 12.0 9.0 13.4

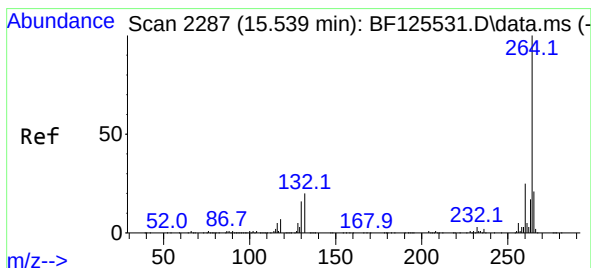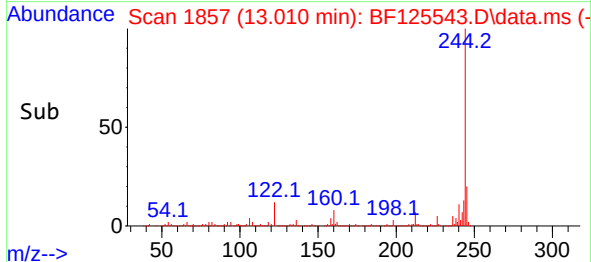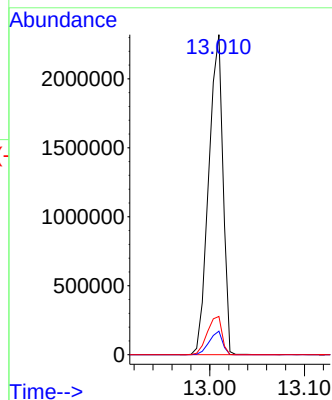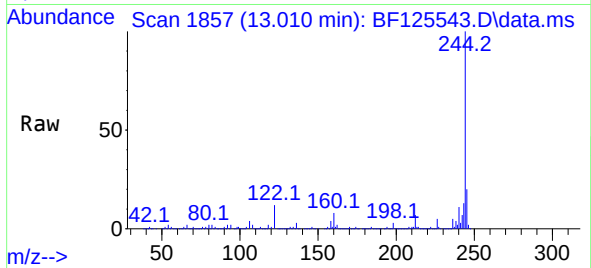

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.533 min Scan# 2286
Delta R.T. -0.006 min
Lab File: BF125543.D
Acq: 21 Sep 2021 19:07

Tgt Ion:264 Resp: 399981
Ion Ratio Lower Upper
264 100
260 24.0 19.6 29.4
265 21.2 17.2 25.8

