
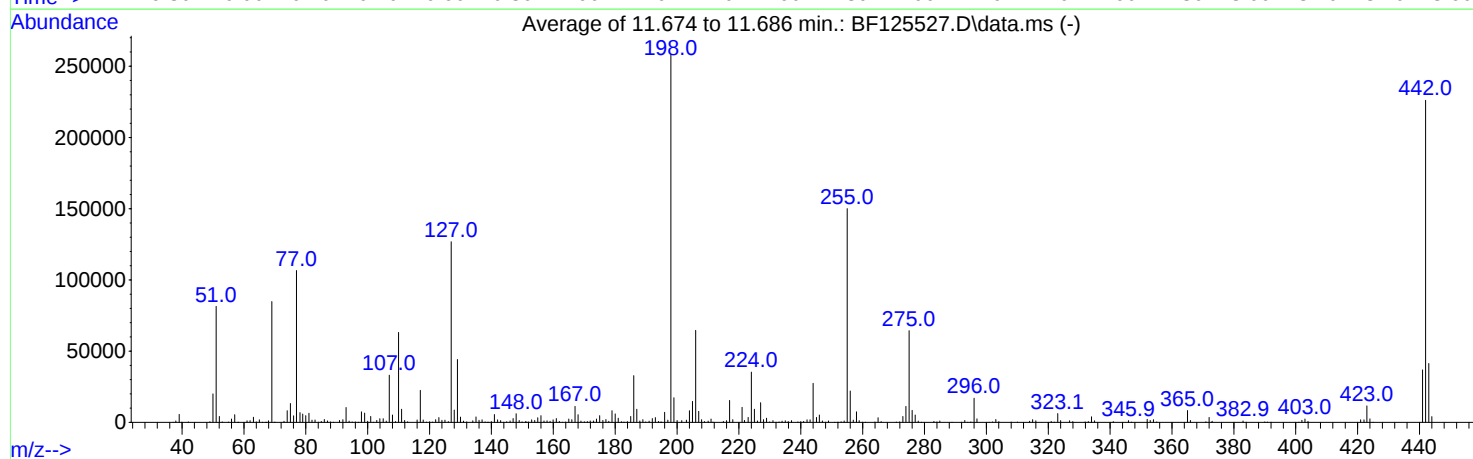


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092121\
 Data File : BF125527.D
 Acq On : 21 Sep 2021 9:42
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 21 19:21:36 2021

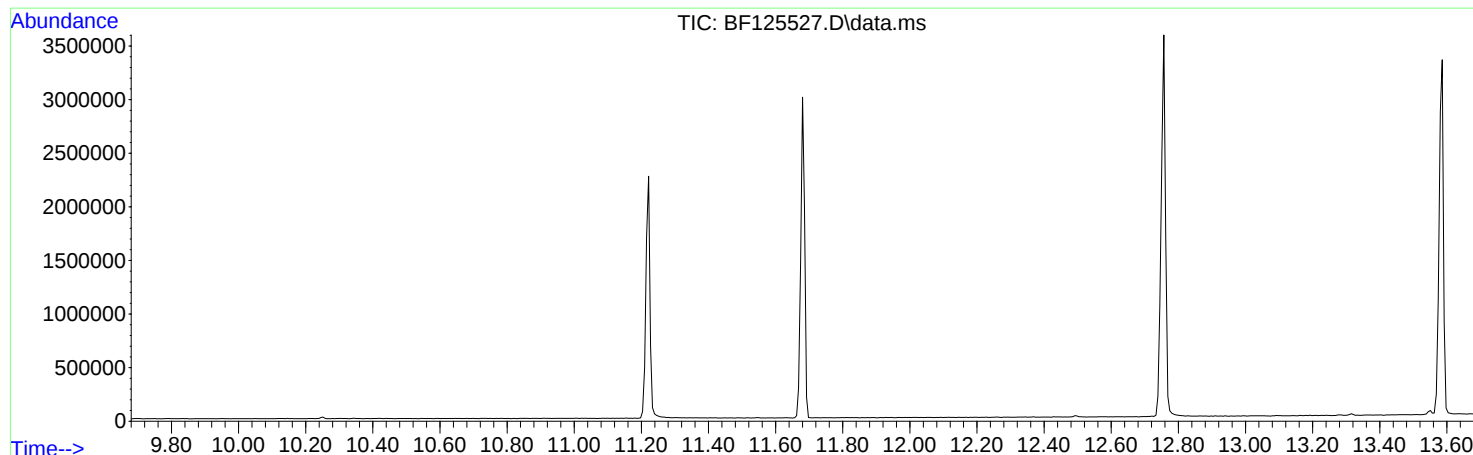




AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	81397	PASS
68	69	0.00	2	1.4	1171	PASS
69	198	0.00	100	32.9	84877	PASS
70	69	0.00	2	0.3	267	PASS
127	198	10	80	49.1	126800	PASS
197	198	0.00	2	0.6	1522	PASS
198	198	100	100	100.0	258261	PASS
199	198	5	9	6.7	17332	PASS
275	198	10	60	24.9	64379	PASS
365	198	1	100	3.2	8347	PASS
441	198	0.01	100	14.3	36892	PASS
442	442	50	100	100.0	226163	PASS
443	442	15	24	18.3	41373	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092121\
 Data File : BF125527.D
 Acq On : 21 Sep 2021 9:42
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 21 12:49:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 21 12:45:25 2021
 Response via : Initial Calibration

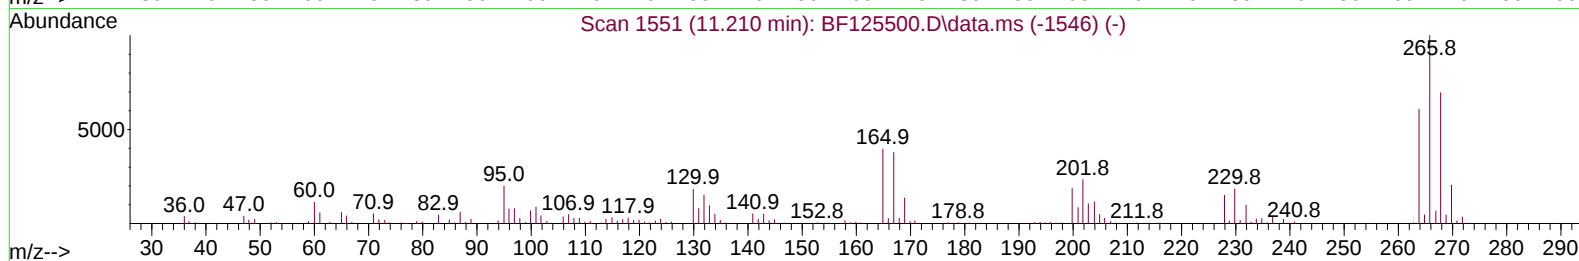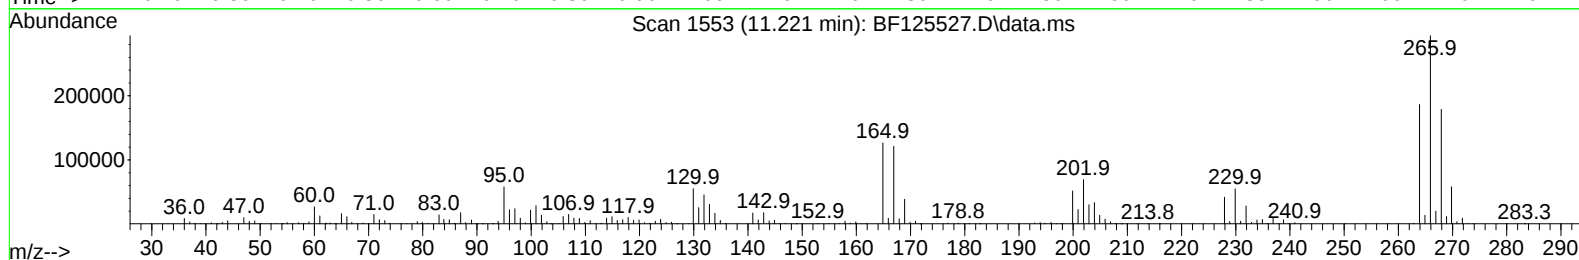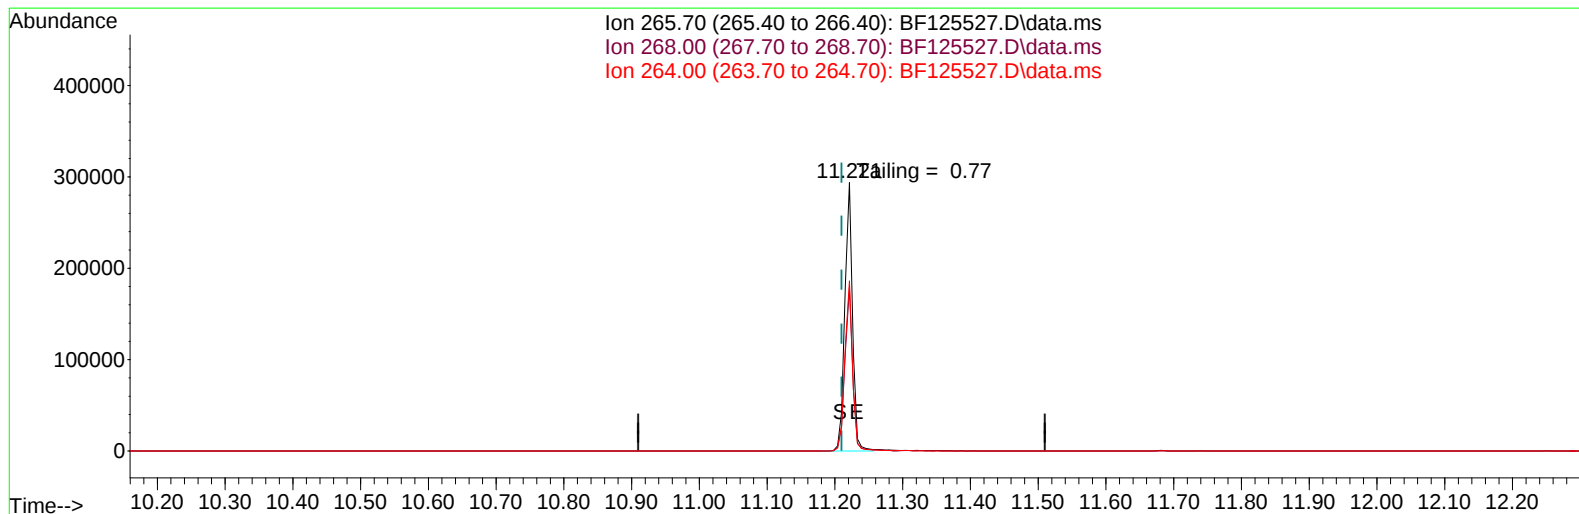

TIC: BF125527.D\data.ms

(70) Pentachlorophenol (C)

11.221min (+ 0.012) 0.00 ng




response 234892

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	60.88
264.00	69.90	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092121\
 Data File : BF125527.D
 Acq On : 21 Sep 2021 9:42
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 21 12:49:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 21 12:45:25 2021
 Response via : Initial Calibration

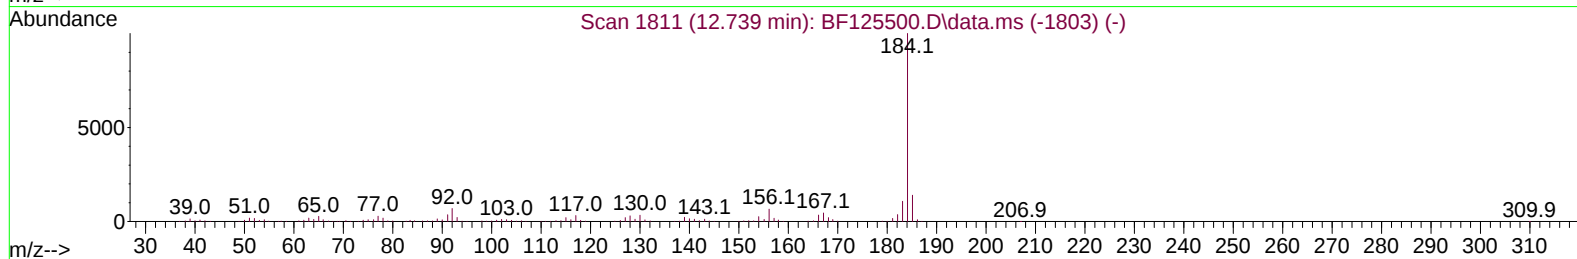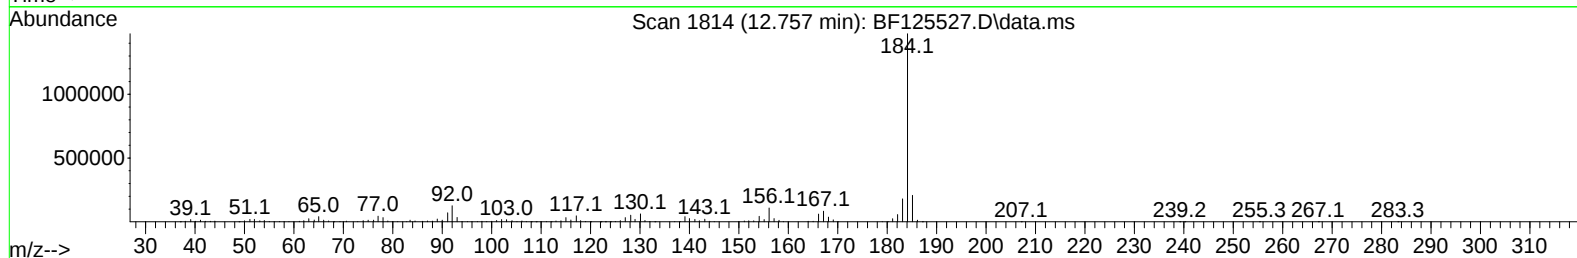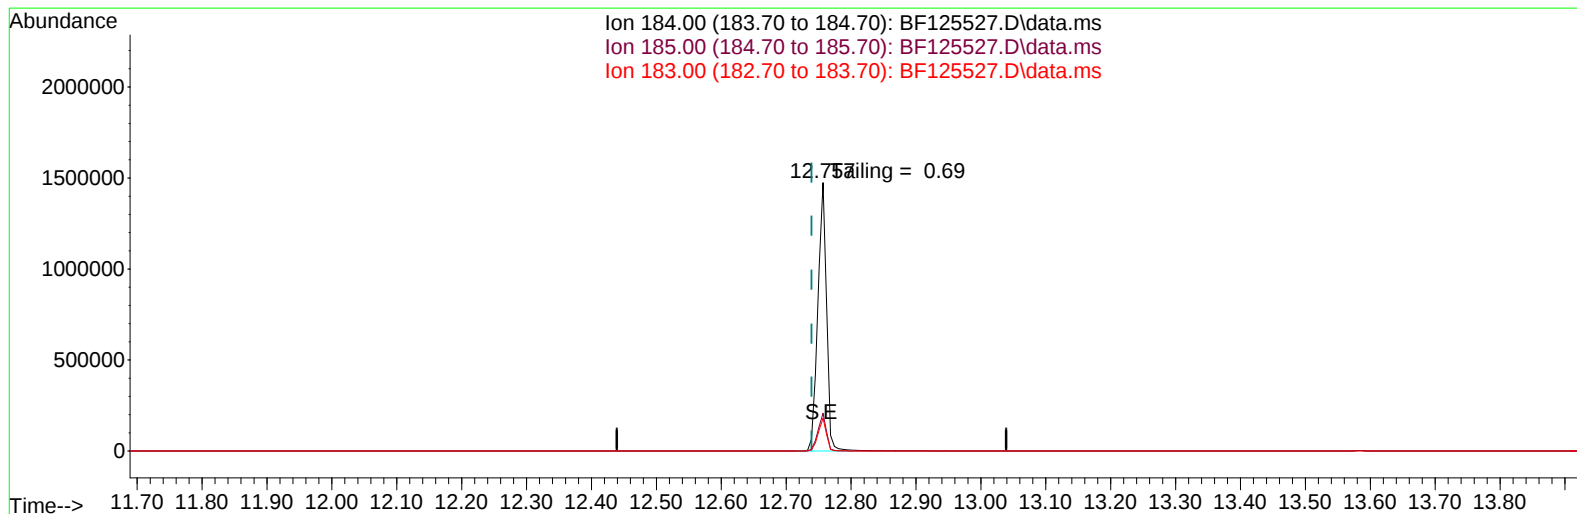

TIC: BF125527.D\data.ms

(77) Benzidine

12.757min (+ 0.018) 202540.19 ng

response 1392459

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.07
183.00	10.10	12.22#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/21/2021	BNA_F	<u>BF125527.D</u>
Compound Name	Response	Retention Time
DDT	557164	13.58
DDD	1064	13.28
DDE	0	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1064	558228	0.19