

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092122\
 Data File : BF130358.D
 Acq On : 21 Sep 2022 13:01
 Operator : CG\JU
 Sample : PB147377BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147377BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130358.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.869	468	473	486	rBV	264704	454399	7.62%	1.290%
2	5.275	536	542	545	rBV	4242513	4754993	79.74%	13.499%
3	6.304	711	717	720	rBV	3802511	4605164	77.22%	13.073%
4	6.651	773	776	780	rBV	967069	894098	14.99%	2.538%
5	7.228	867	874	876	rBV	2702733	3208171	53.80%	9.108%
6	7.940	989	995	998	rBV	1182736	1215968	20.39%	3.452%
7	9.022	1172	1179	1181	rBV	5426421	5963455	100.00%	16.929%
8	9.686	1286	1292	1296	rBV	1562763	1352603	22.68%	3.840%
9	10.481	1420	1427	1430	rBV	4274637	3828502	64.20%	10.869%
10	11.169	1540	1544	1547	rBV	1613441	1288997	21.61%	3.659%
11	12.763	1809	1815	1818	rBV	6631096	5954463	99.85%	16.904%
12	13.798	1987	1991	1995	rBV	1140576	942086	15.80%	2.674%
13	13.898	2003	2008	2012	rBV	61699	77706	1.30%	0.221%
14	15.192	2223	2228	2232	rBV	573012	684820	11.48%	1.944%




Sum of corrected areas: 35225425

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092122\
Data File : BF130358.D
Acq On : 21 Sep 2022 13:01
Operator : CG\JU
Sample : PB147377BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147377BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

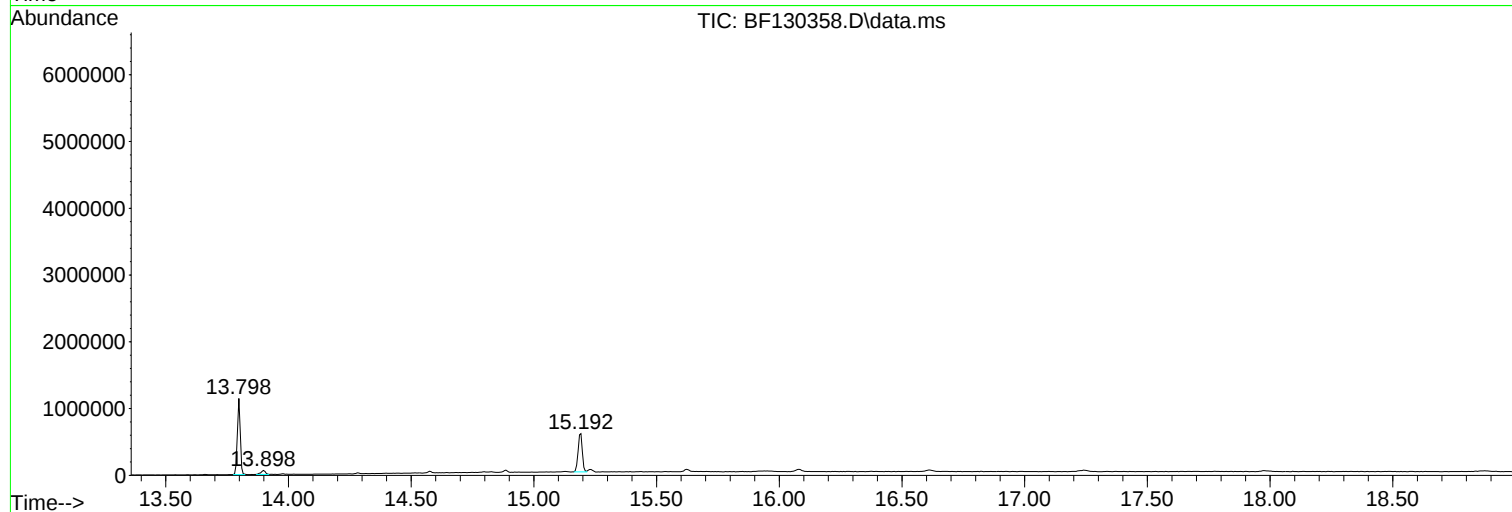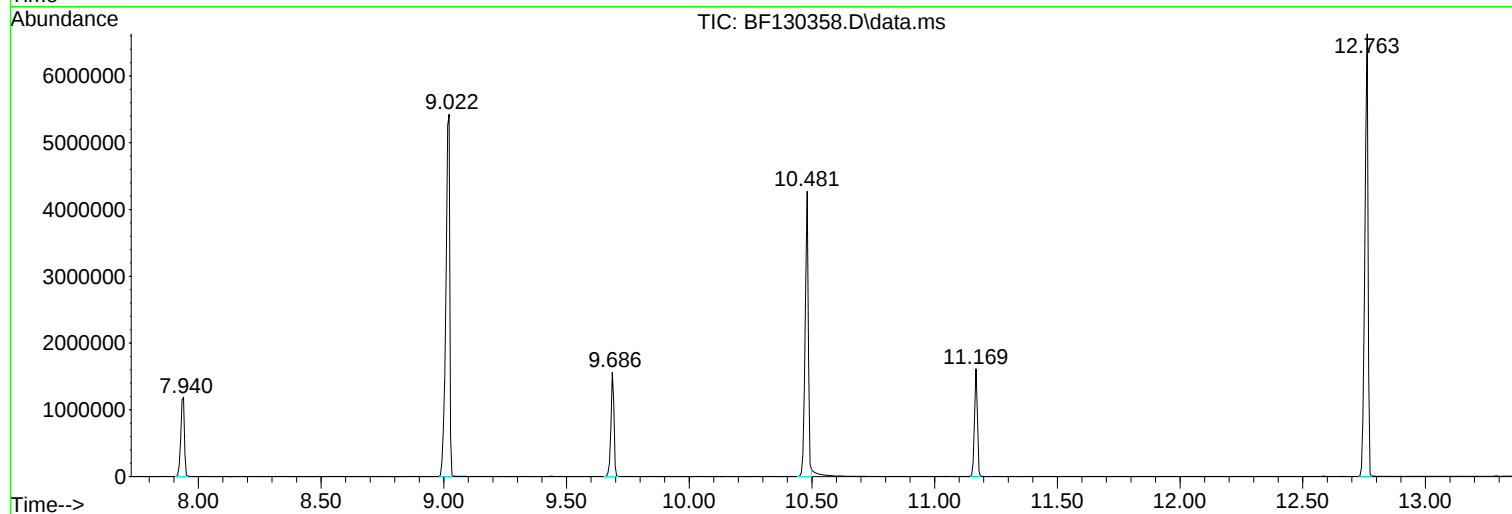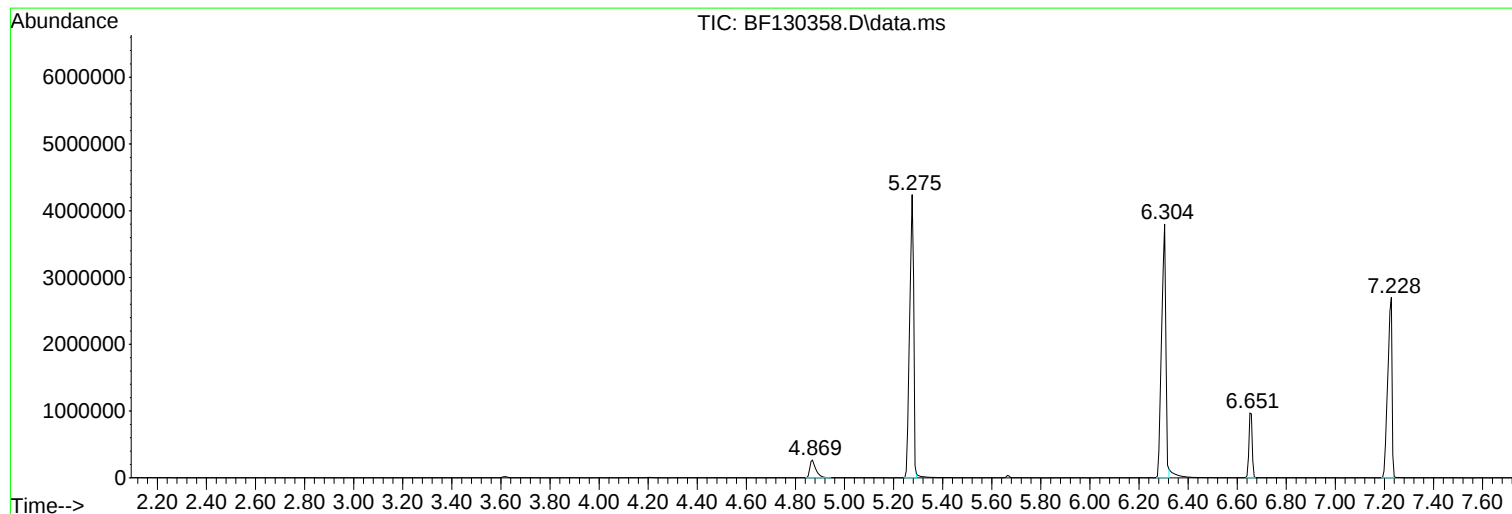

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092122\
Data File : BF130358.D
Acq On : 21 Sep 2022 13:01
Operator : CG\JU
Sample : PB147377BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB147377BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
4.869	10.16 ng	454399	1,4-Dichlorobenzene-d4		6.657	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	56
2	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	10
3	Propanoic acid, 2-nitro-, methyl...		133	C4H7NO4	006118-50-9	9
4	2-Hexanol, 2-methyl-		116	C7H16O	000625-23-0	9
5	Propane, 1-ethoxy-2-methyl-		102	C6H14O	000627-02-1	9

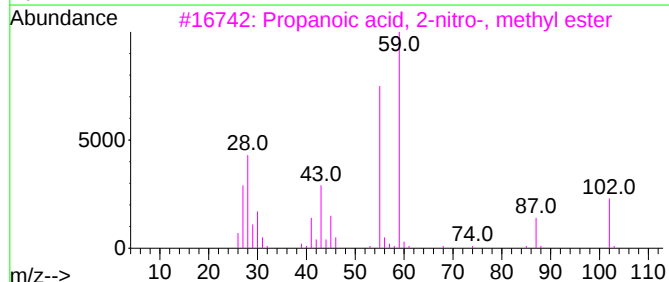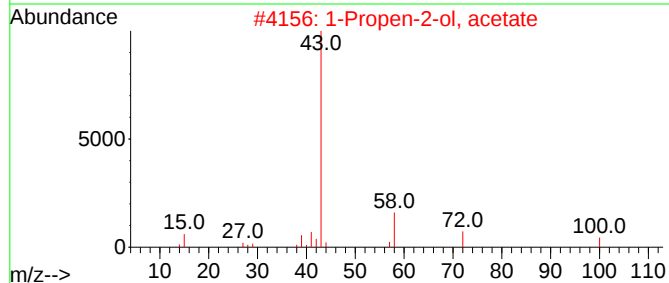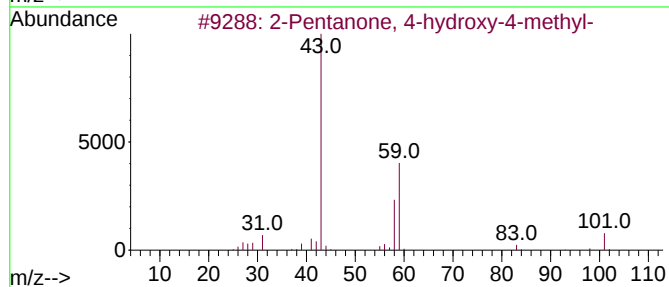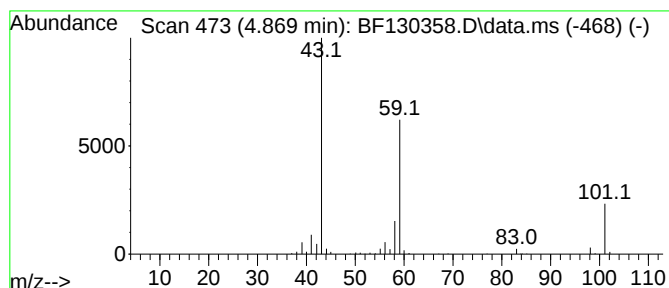

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092122\
Data File : BF130358.D
Acq On : 21 Sep 2022 13:01
Operator : CG\JU
Sample : PB147377BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147377BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.869	10.2	ng	454399	1	6.657	894098	20.0