


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092122\
 Data File : BF130356.D
 Acq On : 21 Sep 2022 11:53
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 19 15:06:14 2022

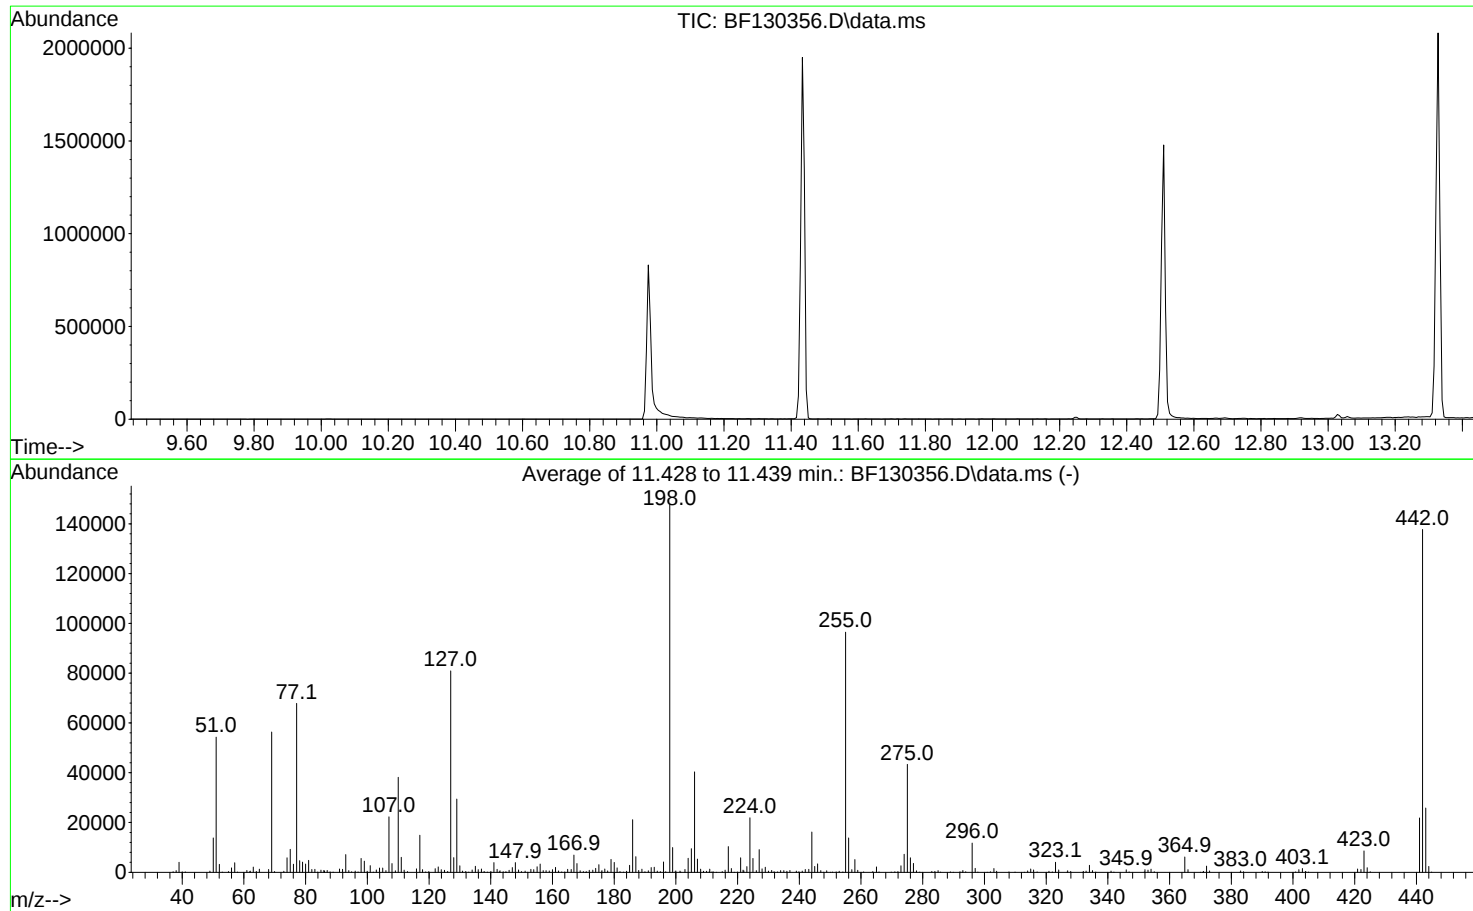




AutoFind: Scans 1588, 1589, 1590; Background Corrected with Scan 1583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	54256	PASS
68	69	0.00	2	2.0	1104	PASS
69	198	0.00	100	38.1	56360	PASS
70	69	0.00	2	0.6	315	PASS
127	198	10	80	54.8	80920	PASS
197	198	0.00	2	0.2	229	PASS
198	198	100	100	100.0	147781	PASS
199	198	5	9	6.7	9910	PASS
275	198	10	60	29.3	43352	PASS
365	198	1	100	4.1	6129	PASS
441	198	0.01	100	14.8	21846	PASS
442	442	50	100	100.0	137741	PASS
443	442	15	24	18.8	25827	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092122\
Data File : BF130356.D
Acq On : 21 Sep 2022 11:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 21 14:01:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 15:06:14 2022
Response via : Initial Calibration

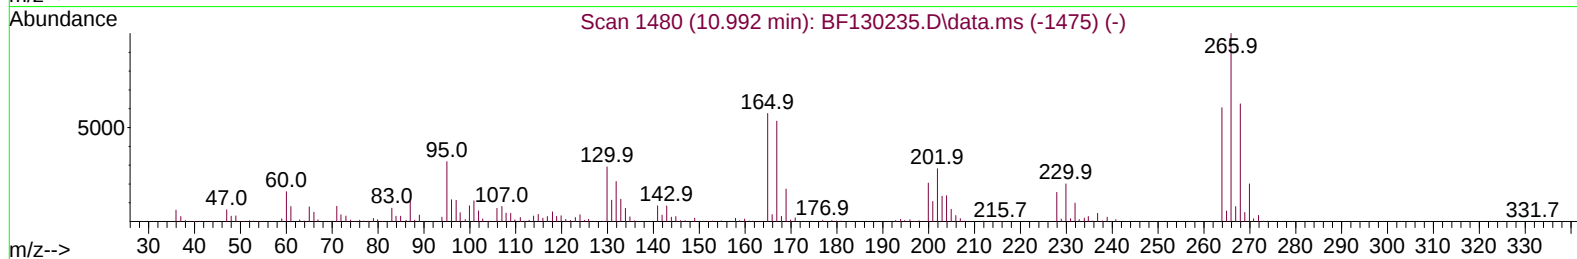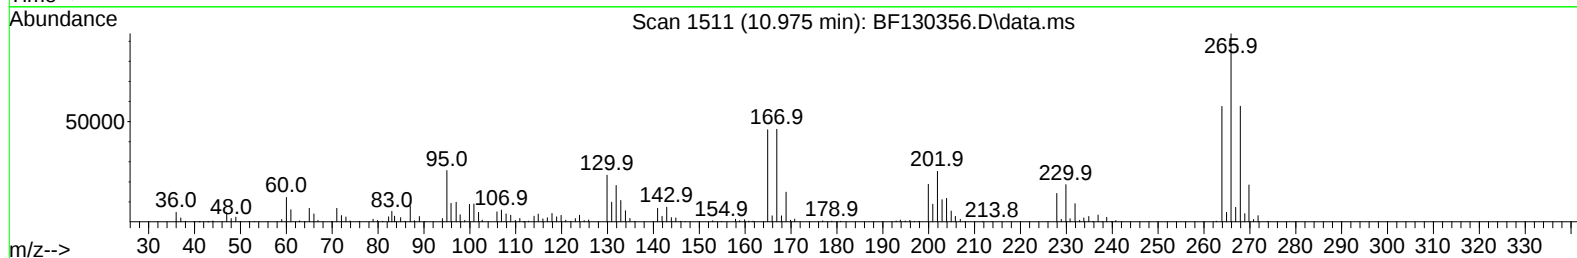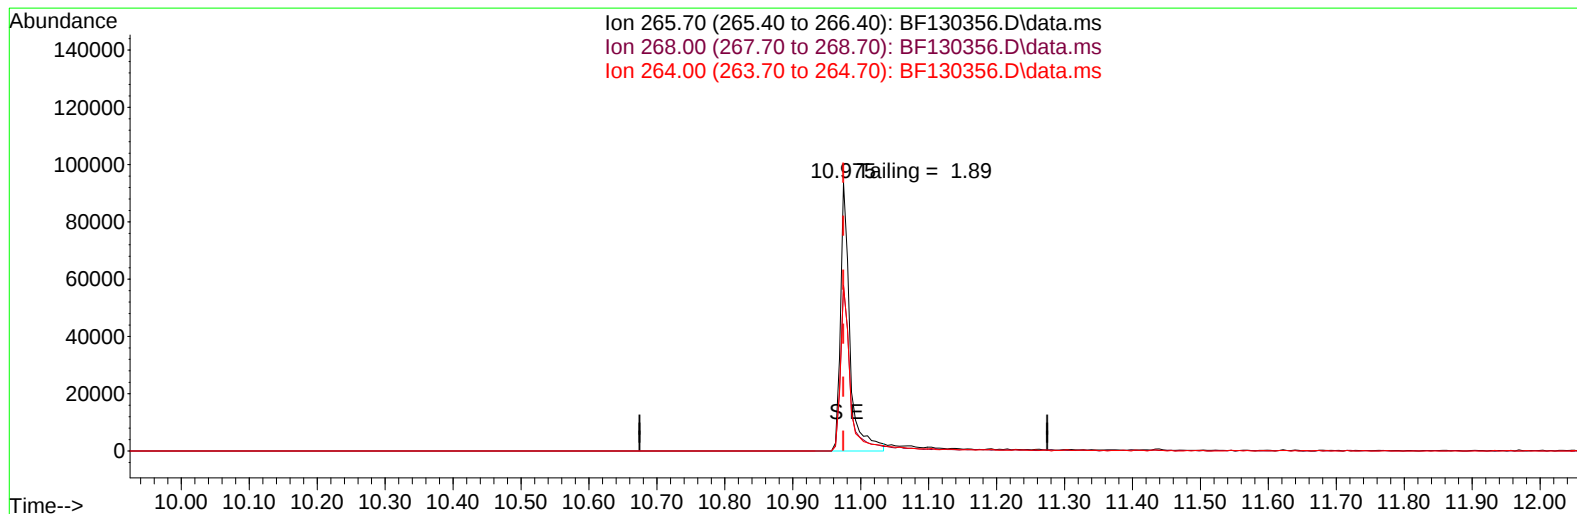

TIC: BF130356.D\data.ms

(70) Pentachlorophenol (C)

10.975min (+ 0.000) 18075.71 ng




response 93289

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	61.54
264.00	63.10	61.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092122\
Data File : BF130356.D
Acq On : 21 Sep 2022 11:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 21 14:01:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 15:06:14 2022
Response via : Initial Calibration

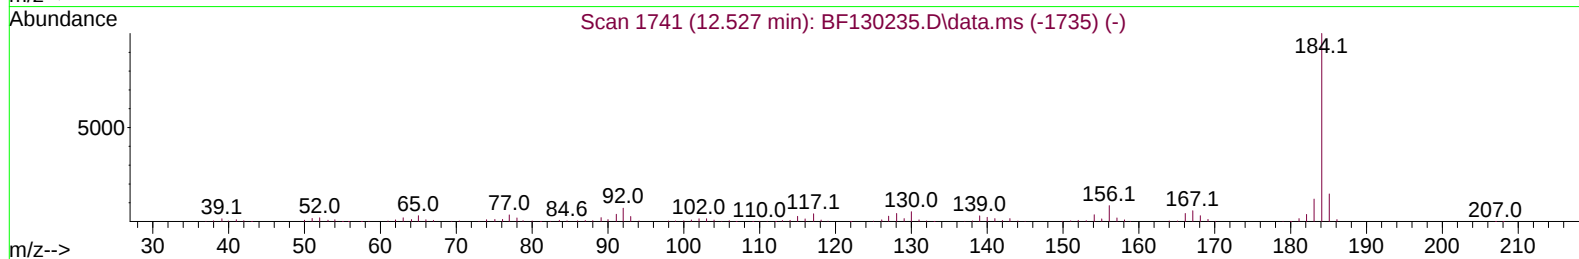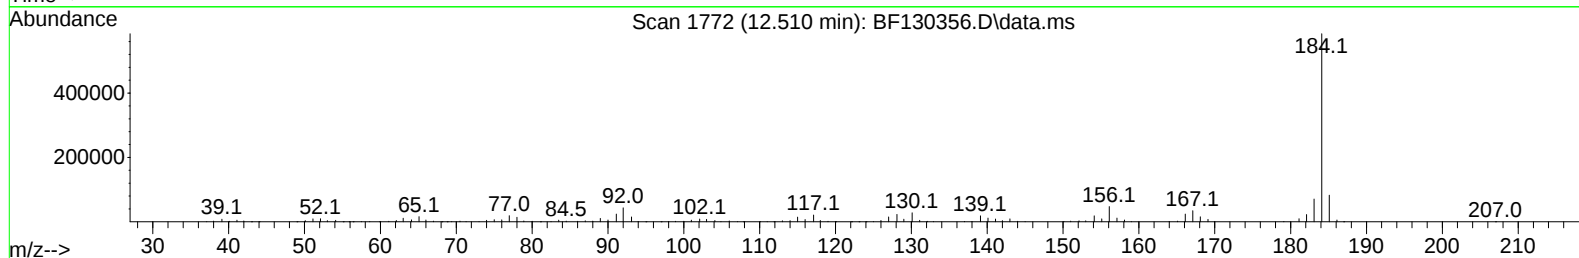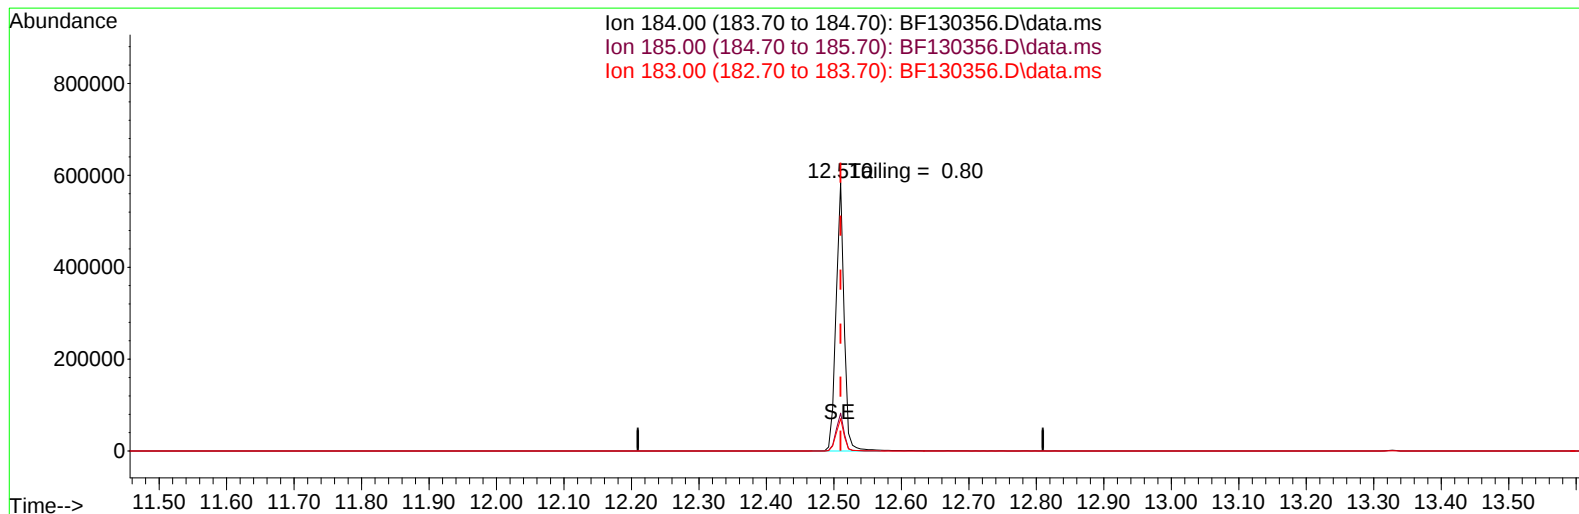

TIC: BF130356.D\data.ms

(77) Benzidine

12.510min (+ 0.000) 0.00 ng

response 485647

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.17
183.00	11.40	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/21/2022	BNA_F	<u>BF130356.D</u>
Compound Name	Response	Retention Time
DDT	317061	13.32
DDD	3706	13.02
DDE	659	12.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4365	321426	1.36

Instrument :
BNA_F
ClientSampleId :
DFTPP