
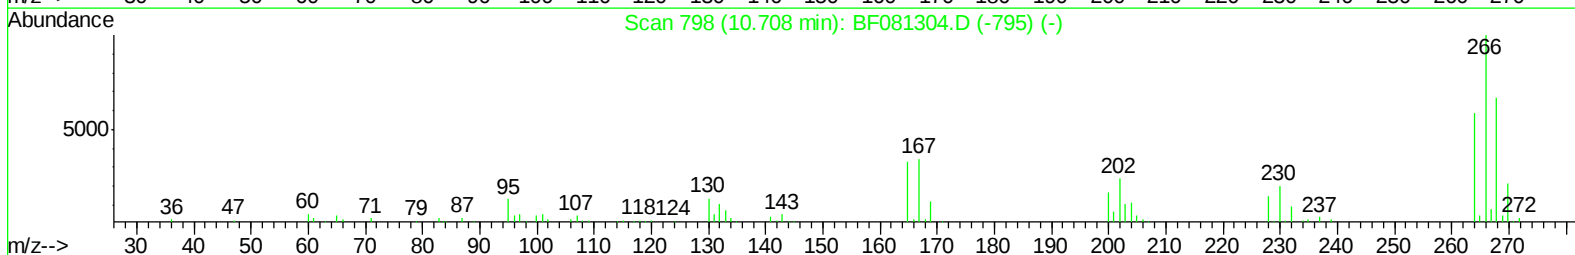
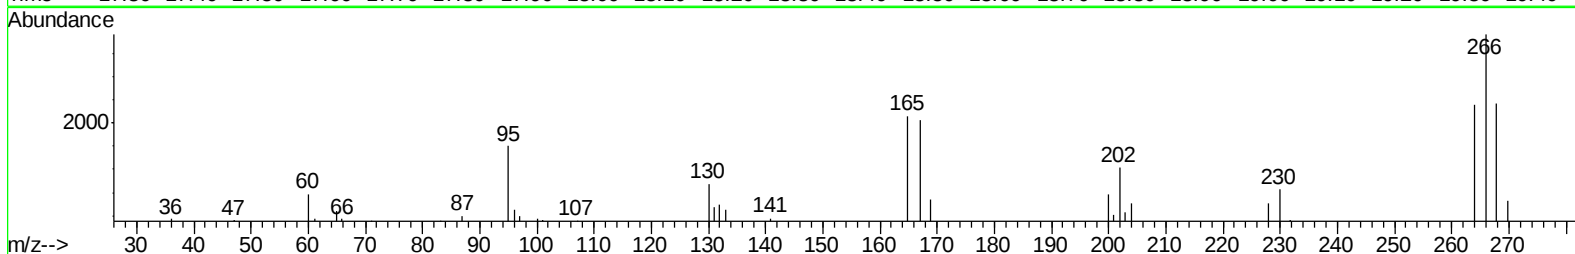


Data Path : Z:\HPCHEM1\BNA_F\Data\BF092215\
Data File : BF081740.D
Acq On : 22 Sep 2015 12:19
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 12:52:38 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 15 14:03:59 2015
Response via : Initial Calibration

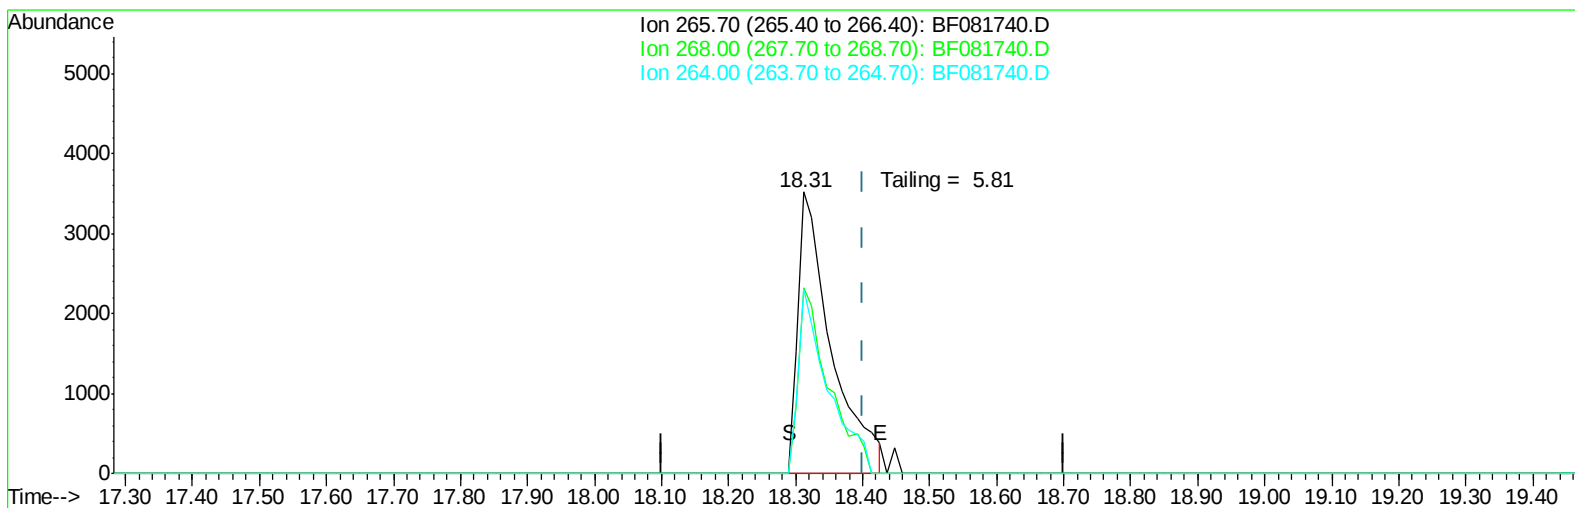

TIC: BF081740.D

(69) Pentachlorophenol (C)




18.311min (-0.090) 0.00ng

response 12459

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	66.11
264.00	62.70	65.65
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF092215\
Data File : BF081740.D
Acq On : 22 Sep 2015 12:19
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 12:52:38 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 15 14:03:59 2015
Response via : Initial Calibration

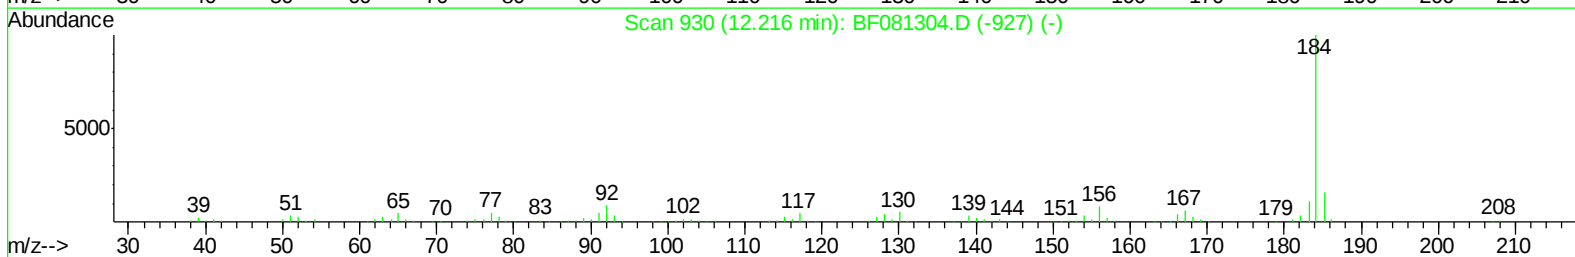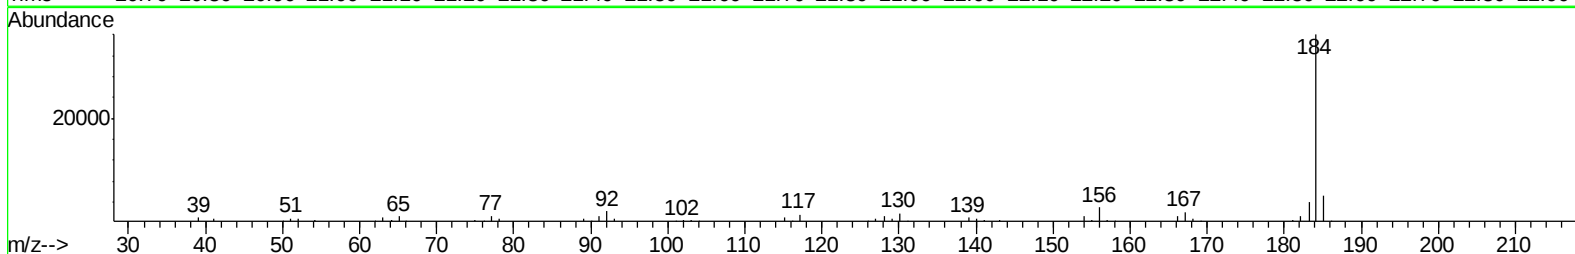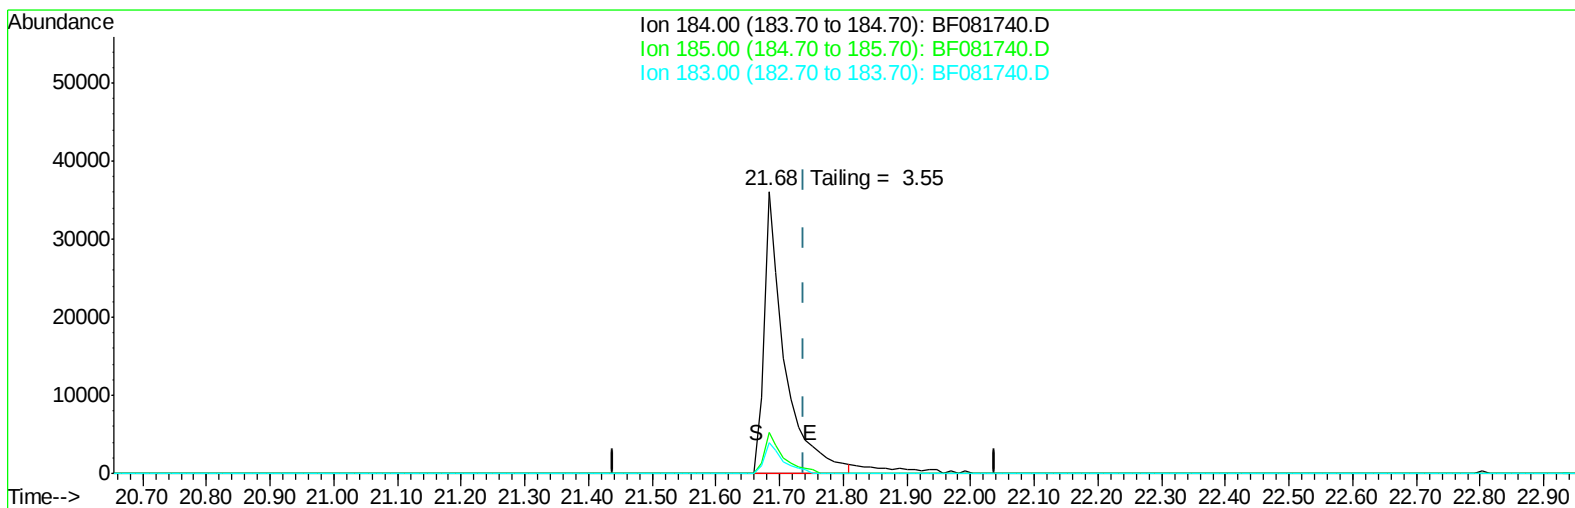

TIC: BF081740.D

(76) Benzidine

21.683min (-0.056) 0.00ng

response 85951

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.48
183.00	9.50	10.94
0.00	0.00	0.00