
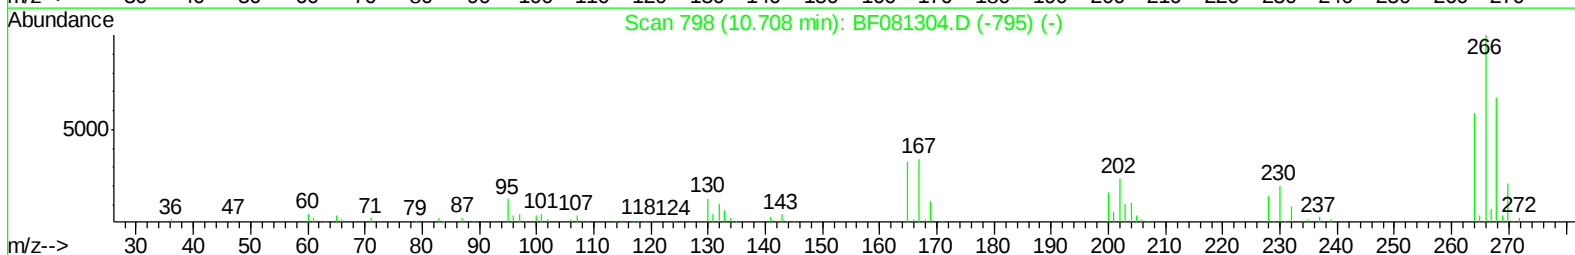
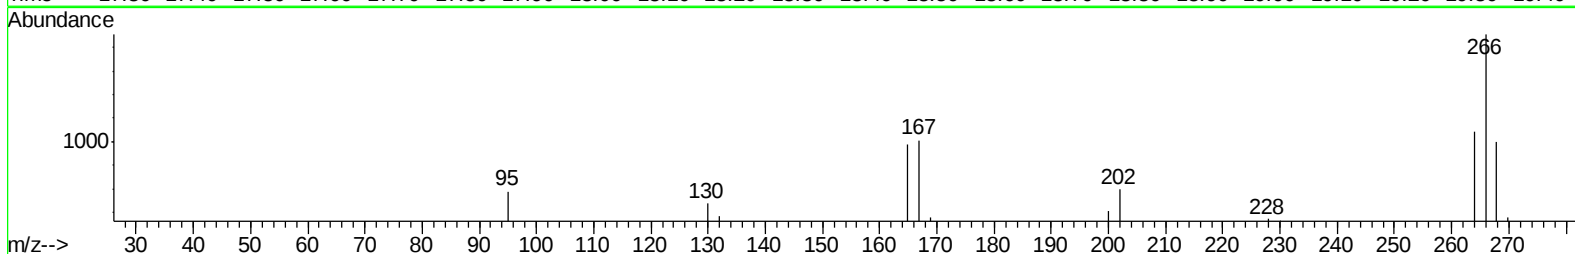


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092215\
Data File : BF081755.D
Acq On : 23 Sep 2015 4:33
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 07:24:28 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 22 17:42:58 2015
Response via : Initial Calibration

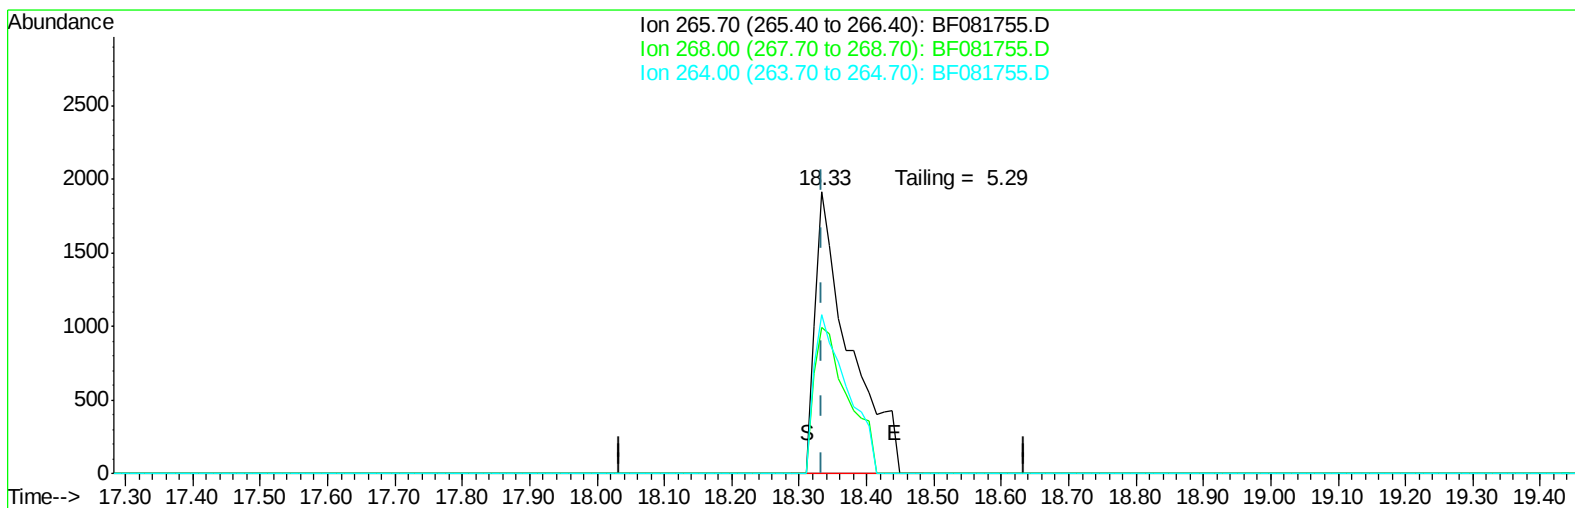

TIC: BF081755.D

(69) Pentachlorophenol (C)




18.334min (+0.000) 0.00ng

response 6596

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	52.01
264.00	62.70	56.56
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092215\
Data File : BF081755.D
Acq On : 23 Sep 2015 4:33
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 07:24:28 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 22 17:42:58 2015
Response via : Initial Calibration

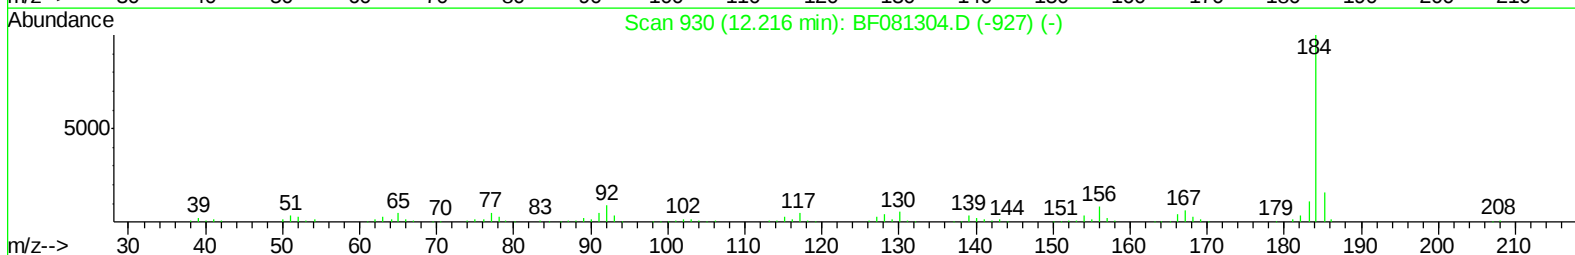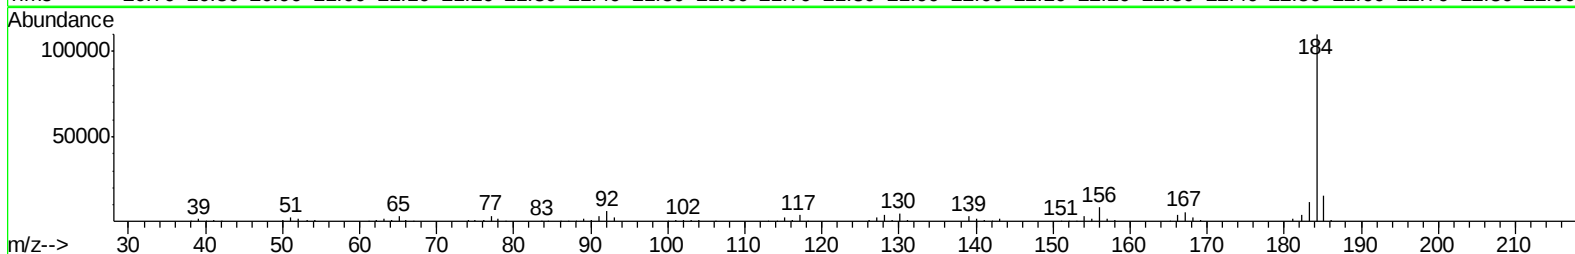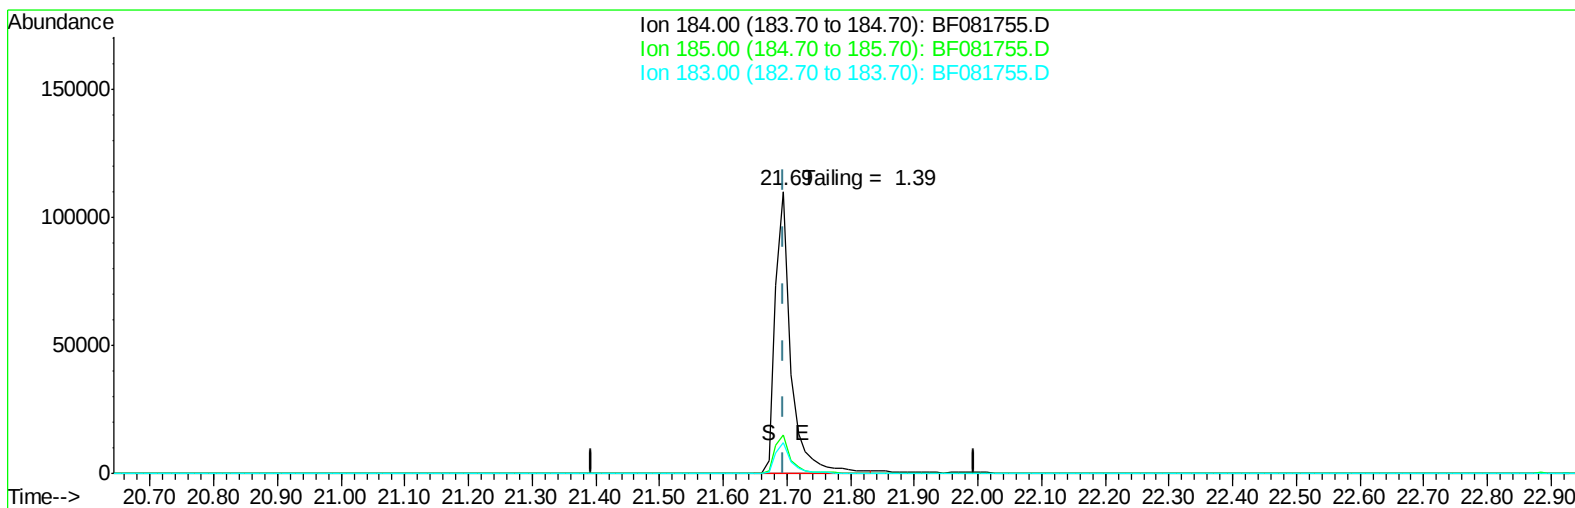

TIC: BF081755.D

(76) Benzidine

21.695min (+0.000) 2762.21ng

response 190436

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.66
183.00	9.50	10.79
0.00	0.00	0.00