


Data Path : Z:\HPCHEM1\BNA F\DATA\BF092215\  
 Data File : BF081740.D  
 Acq On : 22 Sep 2015 12:19  
 Operator : UM/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF090115.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Sep 22 17:42:58 2015

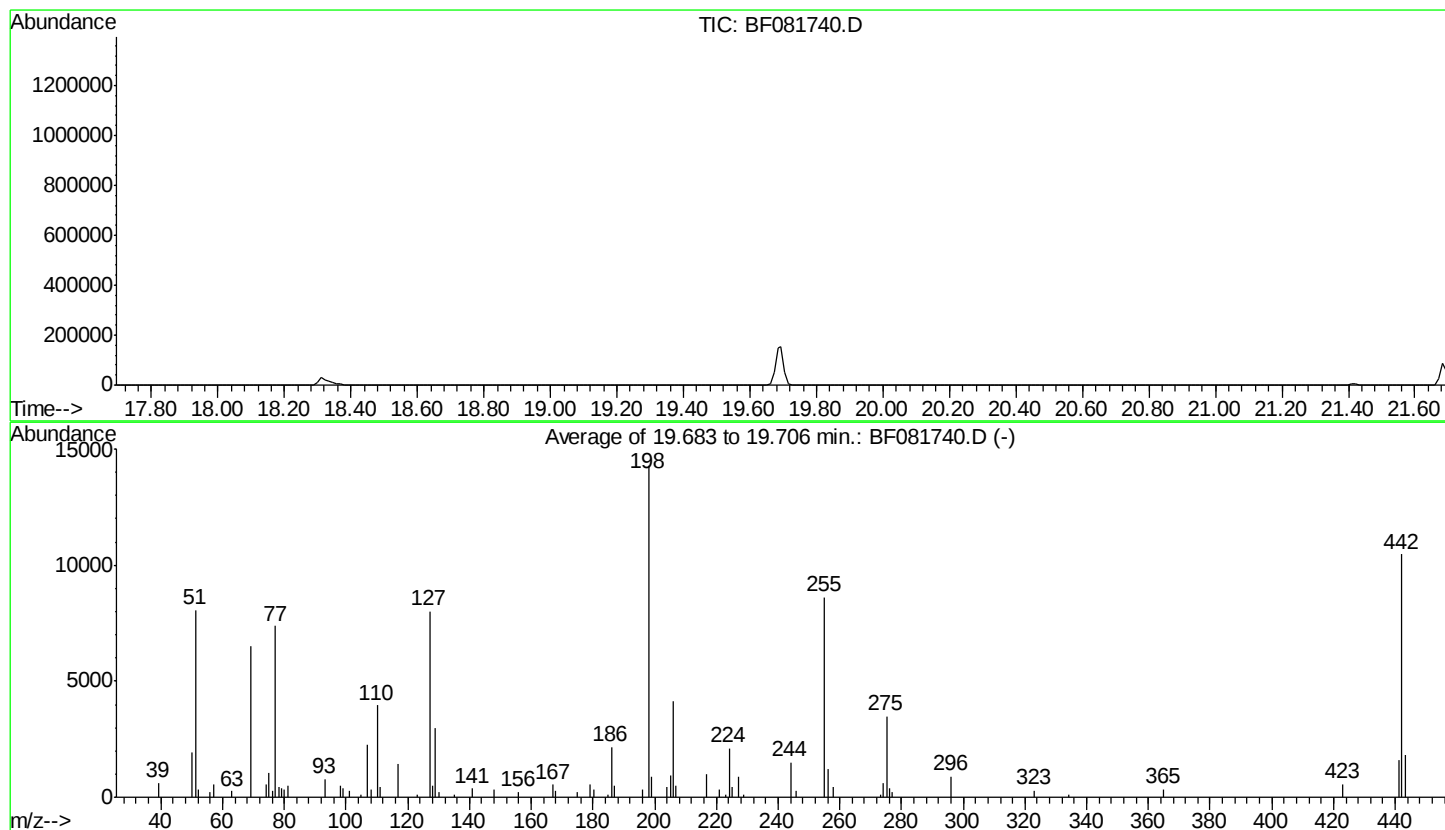

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 56.5      | 8076    | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 45.6      | 6510    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 56.1      | 8012    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 14289   | PASS             |
| 199         | 198          | 5            | 9            | 6.3       | 898     | PASS             |
| 275         | 198          | 10           | 60           | 24.5      | 3501    | PASS             |
| 365         | 198          | 1            | 100          | 2.3       | 335     | PASS             |
| 441         | 442          | 0.01         | 24           | 15.4      | 1609    | PASS             |
| 442         | 198          | 50           | 100          | 73.3      | 10478   | PASS             |
| 443         | 442          | 15           | 24           | 17.6      | 1843    | PASS             |