


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092215\
 Data File : BF081755.D
 Acq On : 23 Sep 2015 4:33
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 22 17:42:58 2015

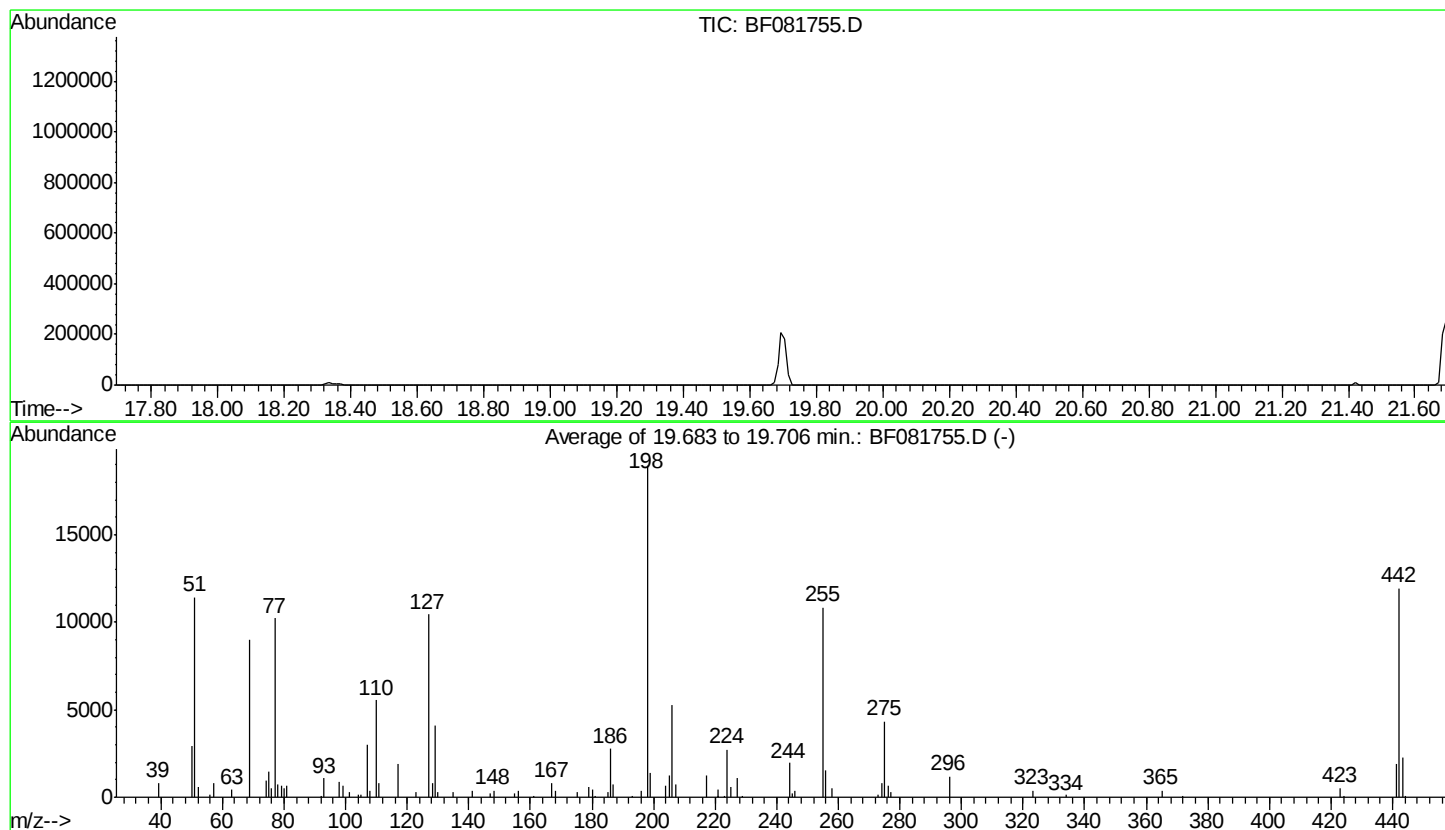

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.4	11434	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.6	9024	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.2	10450	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18941	PASS
199	198	5	9	7.2	1366	PASS
275	198	10	60	22.9	4345	PASS
365	198	1	100	2.1	399	PASS
441	442	0.01	24	16.2	1932	PASS
442	198	50	100	63.0	11933	PASS
443	442	15	24	19.1	2274	PASS