
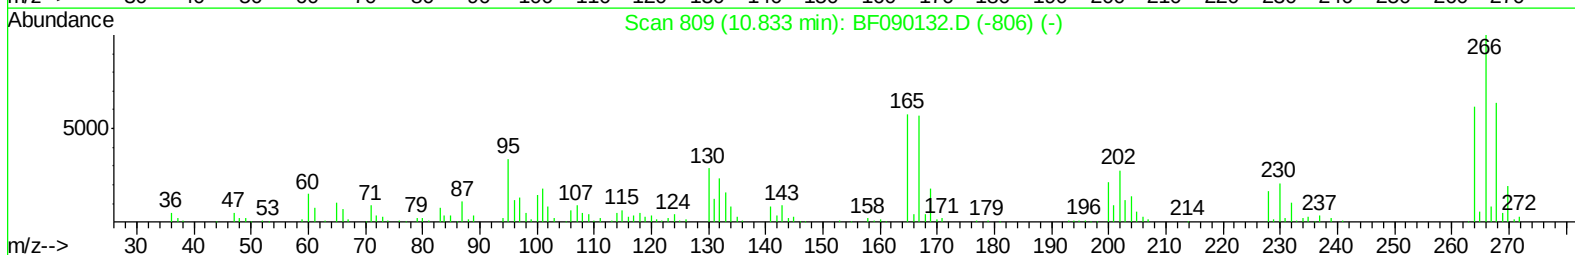
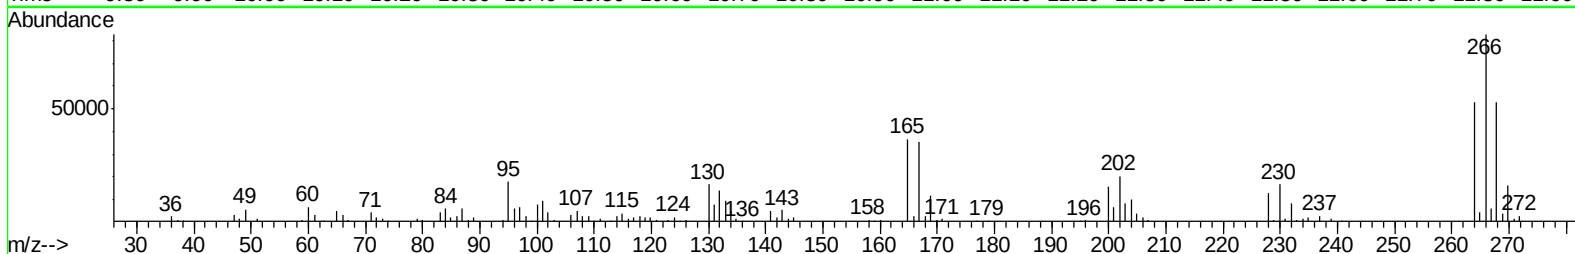


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092216\
Data File : BF090188.D
Acq On : 22 Sep 2016 15:41
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 05:06:38 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 17:58:29 2016
Response via : Initial Calibration

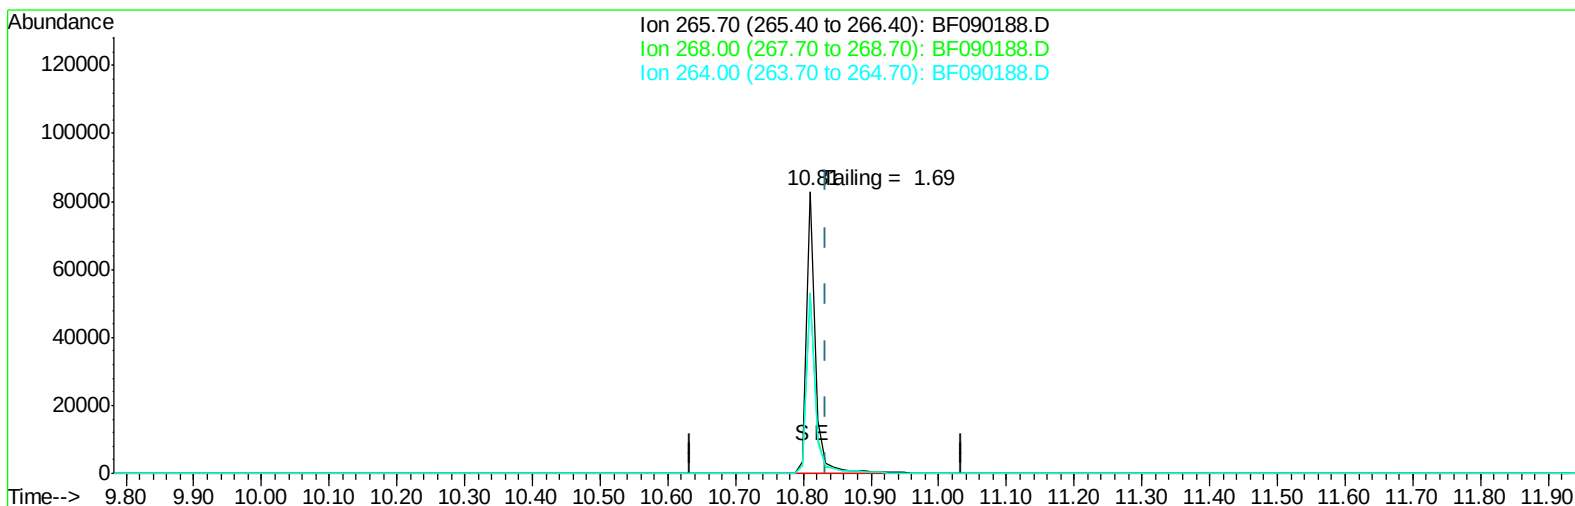

TIC: BF090188.D

(69) Pentachlorophenol (C)




10.811min (-0.023) 21792.07ng

response 77454

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	64.12
264.00	62.90	63.84
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092216\
Data File : BF090188.D
Acq On : 22 Sep 2016 15:41
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 05:06:38 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 17:58:29 2016
Response via : Initial Calibration

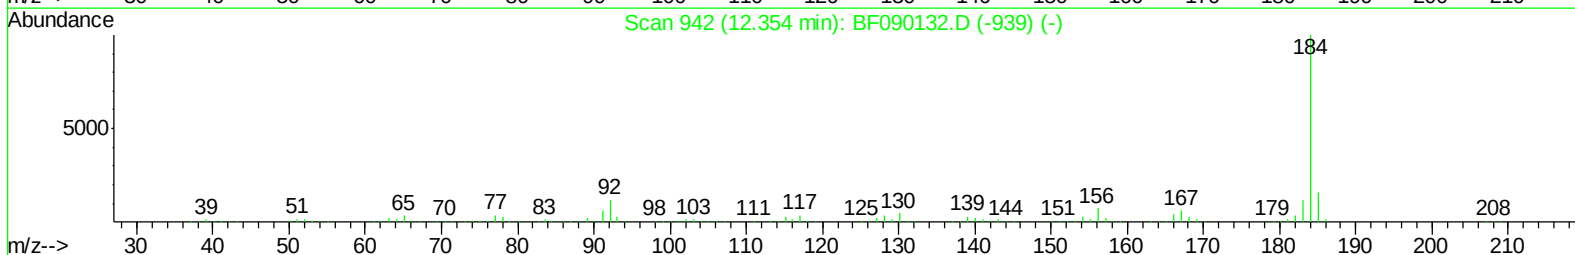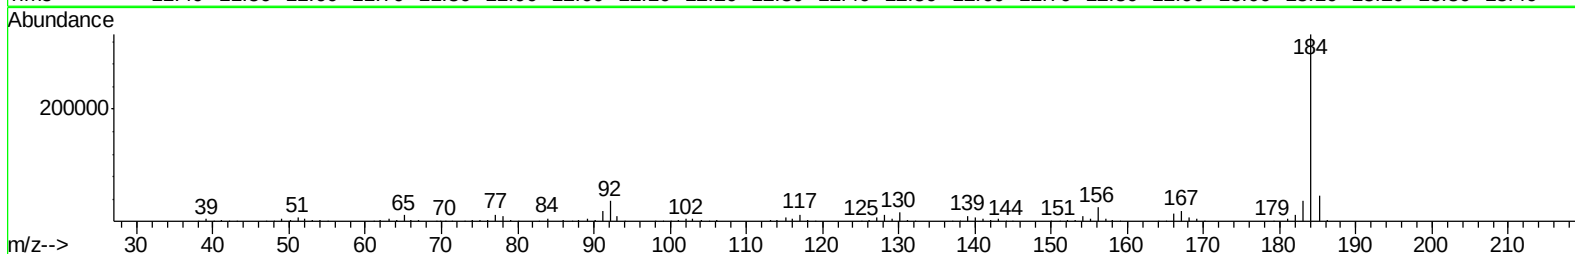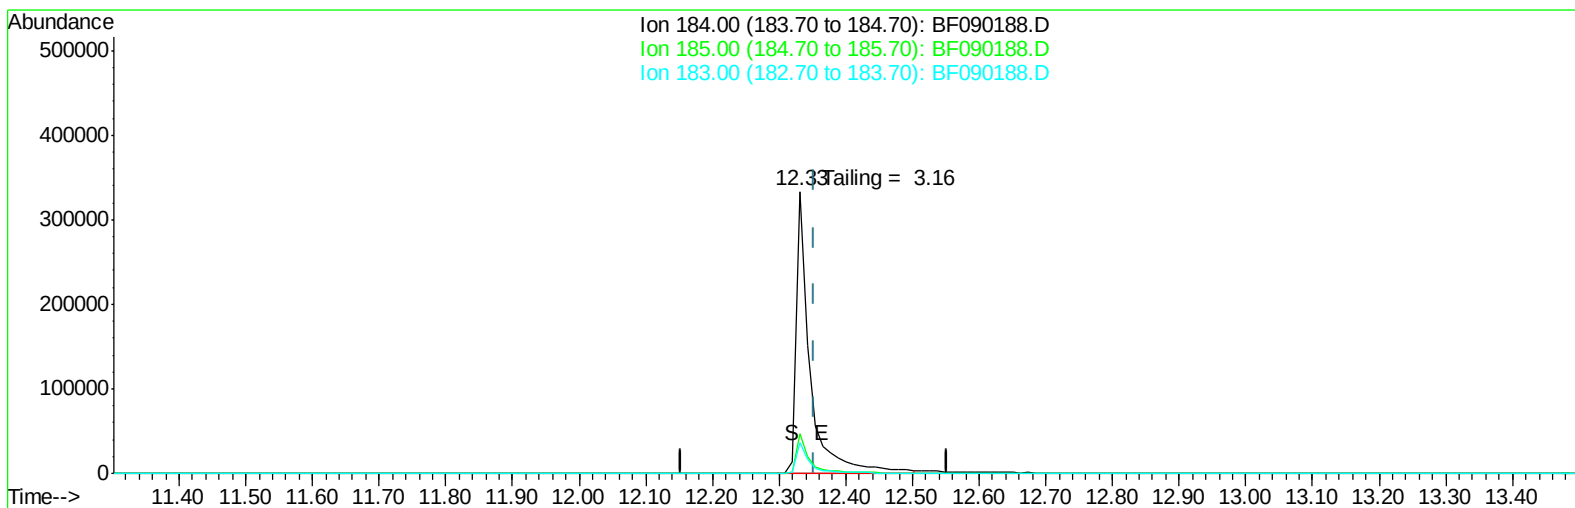

TIC: BF090188.D

(76) Benzidine

12.331min (-0.022) 0.00ng

response 480451

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	13.98
183.00	11.50	11.01
0.00	0.00	0.00