


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092216\
 Data File : BF090188.D
 Acq On : 22 Sep 2016 15:41
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 20 17:58:29 2016

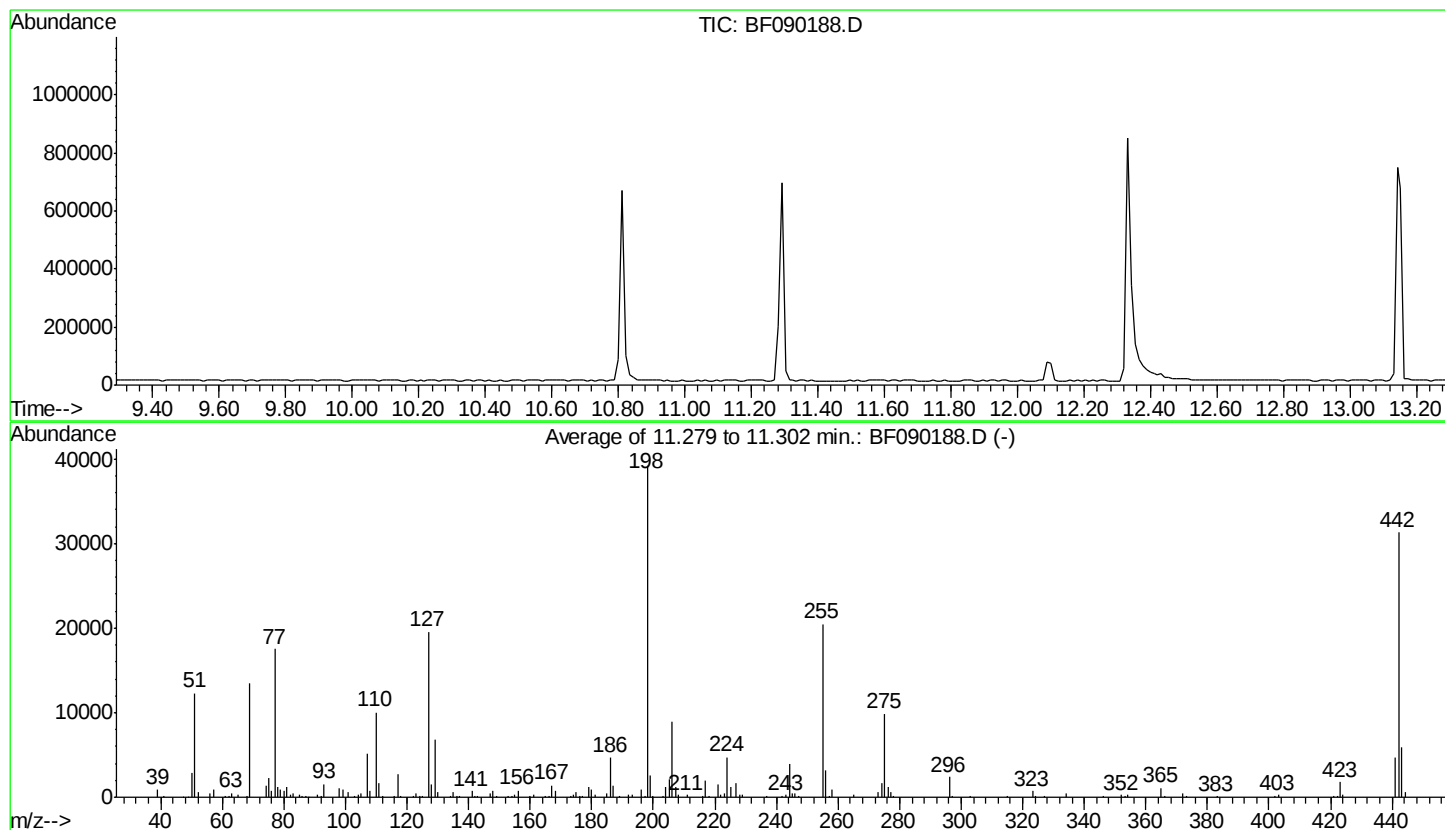

AutoFind: Scans 848, 849, 850; Background Corrected with Scan 845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	12318	PASS
68	69	0.00	2	0.9	120	PASS
69	198	0.00	100	34.5	13510	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.9	19582	PASS
197	198	0.00	2	0.5	180	PASS
198	198	100	100	100.0	39210	PASS
199	198	5	9	6.8	2650	PASS
275	198	10	60	25.2	9875	PASS
365	198	1	100	2.9	1128	PASS
441	442	0.01	24	15.1	4719	PASS
442	198	50	100	79.8	31296	PASS
443	442	15	24	18.8	5883	PASS